LIS01-A2
Vol. 28 No. 13
Replaces LIS1-A
Vol. 23 No. 7

Specification for Low-Level Protocol to Transfer Messages Between Clinical Laboratory Instruments and Computer Systems; Approved Standard—Second Edition

This document describes the electronic transmission of digital information between clinical laboratory instruments and computer systems.

A standard for global application developed through the Clinical and Laboratory Standards Institute consensus process.

CLINICAL AND LABORATORY STANDARDS INSTITUTE®
(Formerly NCCLS)

Clinical and Laboratory Standards Institute

Advancing Quality in Health Care Testing

Clinical and Laboratory Standards Institute (CLSI, formerly NCCLS) is an international, interdisciplinary, nonprofit, standards-developing, and educational organization that promotes the development and use of voluntary consensus standards and guidelines within the health care community. It is recognized worldwide for the application of its unique consensus process in the development of standards and guidelines for patient testing and related health care issues. Our process is based on the principle that consensus is an effective and cost-effective way to improve patient testing and health care services.

In addition to developing and promoting the use of voluntary consensus standards and guidelines, we provide an open and unbiased forum to address critical issues affecting the quality of patient testing and health care.

PUBLICATIONS

A document is published as a standard, guideline, or committee report.

Standard A document developed through the consensus process that clearly identifies specific, essential requirements for materials, methods, or practices for use in an unmodified form. A standard may, in addition, contain discretionary elements, which are clearly identified.

Guideline A document developed through the consensus process describing criteria for a general operating practice, procedure, or material for voluntary use. A guideline may be used as written or modified by the user to fit specific needs.

Report A document that has not been subjected to consensus review and is released by the Board of Directors.

CONSENSUS PROCESS

The CLSI voluntary consensus process is a protocol establishing formal criteria for:

- the authorization of a project
- the development and open review of documents
- the revision of documents in response to comments by users
- the acceptance of a document as a consensus standard or guideline.

Most documents are subject to two levels of consensus—"proposed" and "approved." Depending on the need for field evaluation or data collection, documents may also be made available for review at an intermediate consensus level.

Proposed A consensus document undergoes the first stage of review by the health care community as a proposed standard or guideline. The document should receive a wide and thorough technical review, including an overall review of its scope, approach, and utility, and a line-by-line review of its technical and editorial content.

Approved An approved standard or guideline has achieved consensus within the health care community. It should be reviewed to assess the utility of the final document, to ensure attainment of consensus (ie, that comments on earlier versions have been satisfactorily addressed), and to identify the need for additional consensus documents.

Our standards and guidelines represent a consensus opinion on good practices and reflect the substantial agreement by materially affected, competent, and interested parties obtained by following CLSI's established consensus procedures. Provisions in CLSI standards and guidelines may be more or less stringent than applicable regulations. Consequently, conformance to this voluntary consensus document does not relieve the user of responsibility for compliance with applicable regulations.

COMMENTS

The comments of users are essential to the consensus process. Anyone may submit a comment, and all comments are addressed, according to the consensus process, by the committee that wrote the document. All comments, including those that result in a change to the document when published at the next consensus level and those that do not result in a change, are responded to by the committee in an appendix to the document. Readers are strongly encouraged to comment in any form and at any time on any document. Address comments to Clinical and Laboratory Standards Institute, 940 West Valley Road, Suite 1400, Wayne, PA 19087, USA.

VOLUNTEER PARTICIPATION

Health care professionals in all specialties are urged to volunteer for participation in CLSI projects. Please contact us at customerservice@clsi.org or +610.688.0100 for additional information on committee participation.

LIS01-A2
ISBN 1-56238-665-4
Volume 28 Number 13 ISSN 0273-3099

Specification for Low-Level Protocol to Transfer Messages Between Clinical Laboratory Instruments and Computer Systems; Approved Standard—Second Edition

David Chou, MD
Andrzej J. Knafel, PhD
Charles D. Hawker, PhD, MBA, FACB
Ed Heierman, PhD
David A. Lacher, MD, MEd
William Neeley, MD, FACP
Eugene T. Reilly
Richard S. Seaberg, MT(ASCP)

Abstract

CLSI document LIS01-A2—*Specification for Low-Level Protocol to Transfer Messages Between Clinical Laboratory Instruments and Computer Systems; Approved Standard—Second Edition* describes the electronic transmission of digital information between clinical laboratory instruments (those that measure one or more parameters from one or multiple samples) and computer systems (those that are configured to accept instrument results for further processing, storage, reporting, or manipulation).

Clinical and Laboratory Standards Institute (CLSI). *Specification for Low-Level Protocol to Transfer Messages Between Clinical Laboratory Instruments and Computer Systems; Approved Standard—Second Edition*. CLSI document LIS01-A2 (ISBN 1-56238-665-4). Clinical and Laboratory Standards Institute, 940 West Valley Road, Suite 1400, Wayne, Pennsylvania 19087-1898 USA, 2008.

The Clinical and Laboratory Standards Institute consensus process, which is the mechanism for moving a document through two or more levels of review by the health care community, is an ongoing process. Users should expect revised editions of any given document. Because rapid changes in technology may affect the procedures, methods, and protocols in a standard or guideline, users should replace outdated editions with the current editions of CLSI/NCCLS documents. Current editions are listed in the CLSI catalog and posted on our website at www.clsi.org. If your organization is not a member and would like to become one, and to request a copy of the catalog, contact us at: Telephone: 610.688.0100; Fax: 610.688.0700; E-Mail: customerservice@clsi.org; Website: www.clsi.org



Copyright ©2008 Clinical and Laboratory Standards Institute. Except as stated below, neither this publication nor any portion thereof may be adapted, copied, or otherwise reproduced, by any means (electronic, mechanical, photocopying, recording, or otherwise) without prior written permission from Clinical and Laboratory Standards Institute ("CLSI").

CLSI hereby grants permission to each individual member or purchaser to make a single reproduction of this publication for use in its laboratory procedure manual at a single site. To request permission to use this publication in any other manner, contact the Executive Vice President, Clinical and Laboratory Standards Institute, 940 West Valley Road, Suite 1400, Wayne, Pennsylvania 19087-1898, USA.

Suggested Citation

(CLSI. *Specification for Low-Level Protocol to Transfer Messages Between Clinical Laboratory Instruments and Computer Systems; Approved Standard—Second Edition.* CLSI document LIS01-A2. Wayne, PA: Clinical and Laboratory Standards Institute; 2008.)

Approved Standard
April 2003

Approved Standard—Second Edition
April 2008

ISBN 1-56238-665-4
ISSN 0273-3099

Committee Membership

Area Committee on Automation and Informatics

David Chou, MD
Chairholder
University of Washington Medical Center
Seattle, Washington

Andrzej J. Knafel, PhD
Vice-Chairholder
Roche Instrument Center AG
Rotkreuz, Switzerland

Charles D. Hawker, PhD, MBA, FACB
ARUP Laboratories, Inc.
Salt Lake City. Utah

Ed Heierman, PhD
Abbott Diagnostics
Irving, Texas

David A. Lacher, MD, MEd
National Center for Health Statistics
Hyattsville, Maryland

William Neeley, MD, FACP, DABCC
Detroit Medical Center University Laboratories
Detroit, MI

Eugene T. Reilly
FDA Ctr. For Devices/Rad Health
Rockville, MD

Richard S. Seaberg, MT(ASCP)
North Shore University Hospital
Manhasset, New York

Advisors

Michael G. Bissell, MD, PhD, MPH
Ohio State University
Columbus, Ohio

Suzanne H. Butch, MA, MT(ASCP), SB
The University of Michigan
Ann Arbor, Michigan

Randy R. Davis
Siemens Medical Solutions Diagnostics
Bear, Delaware

Al DeStefano
Sysmex America, Inc.
Mundelein, Illinois

Jeffrey A. DuBois, PhD
NOVA Biomedical Corp.
Waltham, Massachusetts

Arden W. Forrey, Jr., PhD, FACB
University of Washington
Seattle, Washington

David A. Herold, MD, PhD
VA (San Diego) Medical Center
San Diego, California

Georg E. Hoffmann, MD
Trillium GmbH
Grafrath, Germany

Stephen Howlett
Beckman Coulter, Inc.
Miami, Florida

Brian Richard Jackson, MD
ARUP Laboratories
Salt Lake City, Utah

Gary W. Kramer, PhD
National Institute of Standards and Technology
Gaithersburg, Maryland

Rodney S. Markin, MD, PhD
Univ. of Nebraska Medical Center
Omaha, Nebraska

Richard A. McPherson, MD
Medical College of Virginia Hospital
Richmond, Virginia

Paul J. Mountain, MSc, MT(ASCP)
Flamborough, Ontario, Canada

David O'Bryan, PhD
Hibernia Consulting
Portsmouth, New Hampshire

Jeff Quint, PhD
Beckman Coulter, Inc.
Brea, California

Hiroshi Sekiya
Olympus America Inc.
Irving, Texas

Russell H. Tomar, MD
Chicago, Illinois

Staff

Clinical and Laboratory Standards Institute
Wayne, Pennsylvania

Lois M. Schmidt, DA
Vice President, Standards Development and Marketing

David E. Sterry, MT(ASCP)
Staff Liaison

Patrice E. Polgar
Project Manager

Melissa A. Lewis
Editor

Acknowledgment

CLSI and the Area Committee on Automation and Informatics gratefully acknowledge the contributions of Ed Heierman, PhD, Abbott Diagnostics; Randy Davis, Siemens Medical Solutions Diagnostics; and Bill Coughlin, BS, MBA, Data Innovations, for their contributions during the revision of the LIS01-A2 consensus standard.

Contents

Abstract i

Committee Membership iii

Foreword vii

1 Scope 1

2 Introduction 1

3 Terminology 1

4 Significance and Use 2

5 Physical Layer for Serial Binary Data Exchange 3

5.1 Overview 3
5.2 Electrical Characteristics 3
5.3 Mechanical Characteristics 5

6 Data Link Layer for Serial Binary Data Exchange 5

6.1 Overview 5
6.2 Establishment Phase (Link Connection) 6
6.3 Transfer Phase 7
6.4 Termination Phase (Link Release) 9
6.5 Error Recovery 9
6.6 Restricted Message Characters 10

7 Physical Layer for TCP/IP Data Exchange 10

7.1 Overview 10
7.2 Electrical Characteristics 10
7.3 Mechanical Characteristics 12

8 Data Link Layer for TCP/IP Data Exchange 12

8.1 Overview 12
8.2 Establishment Phase (Link Connection) 13
8.3 Transfer Phase 14
8.4 Termination Phase (Link Release) 16
8.5 Error Recovery 16
8.6 Restricted Message Characters 17

References 18

Appendix A. Mandatory Information 19

Appendix B. Nonmandatory Information 20

Summary of Delegate Comments and Area Committee Responses 21

The Quality Management System Approach 24

Related CLSI Reference Materials 25

Foreword

In 2001, ASTM Committee E31 decided to restructure its operations, with the intent of focusing on standards-development issues such as security, privacy, and the electronic health record. Part of the reorganization plan was to transfer responsibility for E31.13 standards to CLSI, then known as NCCLS.

Following this transfer, nine standards (formerly ASTM E792; E1029; E1238; E1246; E1381; E1394; E1466; E1639; and E2118) were redesignated as CLSI/NCCLS standards LIS1 through LIS9.[1-8] This collection of standards provides a wide variety of information relating to clinical laboratory computer systems. Some included documents are of general interest as reference sources; others represent specifications of primary importance to instrument manufacturers. LIS2 is a revision of the former ASTM E1381-02.

The Area Committee on Automation and Informatics has assumed responsibility for maintaining the documents and will revise or update each document in accord with the CLSI Administrative Procedures. The area committee prioritized LIS1-A as the second standard from this collection to be updated, incorporated into the CLSI document template, and advanced through the CLSI consensus process. The area committee will revise other documents in the series in a similar manner.

With the transfer of the former ASTM standards, the Area Committee on Automation and Informatics has expanded its mission statement to include laboratory information systems. In the future, the area committee will develop additional standards addressing informatics issues, as well as issues related to the integration of patient clinical data.

This document replaces the first edition of the approved guideline, LIS1-A, which was published in 2003. Several changes were made in this edition; among them, TCP/IP communication is now included (Sections 4.4 and 4.5) and the state diagram was replaced (see Appendix A) so it is consistent with the text of the document.

The revisions in this edition of the LIS01 standard are also intended to delineate this document from its former ASTM edition. The title and text have been revised throughout to indicate that this standard applies to clinical laboratory instruments. The term *computer* has been replaced with the term *information* to better reflect the current terminology (ie, LIS) and the headings of Sections 6 and 8 have been changed to make them more specific.

Key Words

data link layer, physical layer, serial binary data exchange, TCP/IP data exchange

Specification for Low-Level Protocol to Transfer Messages Between Clinical Laboratory Instruments and Computer Systems; Approved Standard—Second Edition

1 Scope

This specification describes the electronic transmission of digital information between clinical laboratory instruments and computer systems.

This specification addresses the low-level protocol used for both serial binary data exchange and TCP/IP data exchange. For message content in the interface between clinical instruments and computer systems, reference CLSI/NCCLS document LIS2.[1]

2 Introduction

The clinical laboratory instruments under consideration are those that measure one or more parameters from one or more patient samples. Often they will be automated instruments that measure many parameters from many patient samples. The computer systems considered here are those that are configured to accept instrument results for further processing, storage, reporting, or manipulation. This instrument output may include patient results, quality control results, and other related information. Typically, the computer system will be a clinical laboratory information management system (CLIMS).

The terminology of the International Organization for Standardization (ISO) Reference Model for Open Systems Interconnection (OSI) is generally followed in describing the communications protocol and services.[9] The electrical and mechanical connection between instrument and computer is described in the Physical Layer sections (see Sections 5 and 7). The methods for establishing communication, error detection, error recovery, and sending and receiving of messages are described in the Data Link Layer sections (see Sections 6 and 8). The data link layer interacts with higher layers in terms of sending and receiving "messages," handles data link connection and release requests, and reports the data link status.

3 Terminology

3.1 **receiver** – the device that responds to the sender and accepts the message.

3.2 **sender** – the device that has a message to send and initiates the transmission process.

3.3 The parts of a communication between instrument and computer are identified by the following terms. The parts are hierarchical and are listed in order of most encompassing first.

3.3.1 **session** – a total unit of communication activity, used in this standard to indicate the events starting with the establishment phase and ending with the termination phase, as described in subsequent sections.

3.3.2 **message** – a collection of related information on a single topic, used here to mean all the identity, tests, and comments sent at one time; **NOTE:** When used with CLSI/NCCLS document LIS2,[1] this term means a record as defined by CLSI/NCCLS document LIS2.[1]

3.3.3 **frame** – a subdivision of a message, used to allow periodic communication housekeeping, such as error checks and acknowledgments.

©*Clinical and Laboratory Standards Institute. All rights reserved.*

4 Significance and Use

4.1 Nearly all recent major clinical instruments have provisions for connection to a computer system, and in nearly all laboratories that have implemented a CLIMS, there is a need to connect the laboratory's high volume automated instruments to the CLIMS, so results can be transferred automatically. To accomplish this connection, both the instrument and the computer must have compatible circuits and appropriate software, and there must be a proper cable to connect the two systems.

4.1.1 Without this standard specification, the interface between each different instrument and each different computer system is likely to be a different product. This increases the cost, the chances for compatibility problems, and the difficulty of specifying and designing a proper system. In addition, interfaces for every instrument-computer combination may not be available, forcing expensive and time-consuming custom development projects.

4.2 This standard specification defines the electrical parameters, cabling, data codes, transmission protocol, and error recovery for the information that passes between the instrument and the laboratory computer. It is expected that future products from instrument manufacturers and computer system developers, released after the publication of this specification, will conform to this specification, and that will lead to plug-together compatibility of clinical instruments and computer systems.

4.3 This standard specification does not define the transmission of character encodings that require greater than eight bits; however, character encodings greater than eight bits can be transmitted through the use of appropriate algorithmic transformations. Examples include using Shift JIS for the transmission of Japanese characters defined by the Japanese Industrial Standards JIS X 0207 (single-byte characters) and JIS X 0208 (double-byte characters), as well as the transmission of the Unicode/UCS-2 character set with a UTF-8 encoding. These techniques do not violate the character-oriented protocol and associated character restrictions described by the data link layer of this standard. There are no provisions in the standard to identify if a specific transmission approach is being used; therefore, the character encoding and transmission approach must be agreed upon outside of the context of this standard.

4.4 This standard specification was originally intended for serial communication between clinical laboratory instruments and computer systems. In order to address bandwidth concerns with serial communication and to address a shift toward the use of networked solution, this standard was updated to include TCP/IP communication as well as frame sizes of 64 000 characters.

4.4.1 It is recommended that the use of large frame sizes be restricted to TCP/IP communication, where the frames will be broken down into smaller packets for transmission. This will ensure proper error detection and recovery for the transmissions.

4.4.2 When the TCP/IP data exchange is used, additional overhead is encountered, because TCP/IP is itself a low-level protocol; and LIS01-A2 protocol activities such as error checking and error recovery are also performed as part of the TCP/IP protocol. In addition, this standard specification is often used in combination with CLSI/NCCLS document LIS2,[1] which defines specific message formats. It may be more appropriate to use CLSI/NCCLS document LIS2[1] directly over TCP/IP, the Health Level Seven Protocol for electronic exchange, or the CLSI/NCCLS standard AUTO3[10] for communication with automated clinical laboratory systems, instruments, devices, and information systems when using the TCP/IP communication protocol to exchange information.

4.5 Although this specification addresses serial communication using a 25-pin connector and TCP/IP communication, it can be adapted to other standard communication approaches such as a 9-pin

 ©*Clinical and Laboratory Standards Institute. All rights reserved.*

serial connector, wireless, high speed USB, and firewire. The physical layer specifications for other approaches must be agreed upon outside the context of this standard. Adaptation to 9-pin, USB, etc. is standard, and can be accomplished in a manner transparent to the specification.

5 Physical Layer for Serial Binary Data Exchange

5.1 Overview

The mechanical and electrical connection for serial binary data bit transmission between instrument and computer system is described in the physical layer. The topology is point-to-point, a direct connection between two devices.

5.2 Electrical Characteristics

The voltage and impedance levels for the generator and receiver circuits are as specified in the EIA-232-D-1986 standard.[11]

5.2.1 Signal Levels

5.2.1.1 For the data interchange circuits, a marking condition corresponds to a voltage more negative than minus three volts with respect to signal ground at the interface point. A spacing condition corresponds to a voltage more positive than plus three volts with respect to signal ground at the interface point.

5.2.1.2 Binary state ONE (1) corresponds to the marking condition; binary state ZERO (0) corresponds to the spacing condition.

5.2.1.3 The signal levels conform to the EIA-232-D-1986 standard.[11]

5.2.2 Character Structure

5.2.2.1 The method of data transmission is serial-by-bit start/stop. The order of the bits in a character is:

(1) One start bit, corresponding to a binary 0;
(2) The data bits of the character, least significant bit transmitted first;
(3) Parity bit; and
(4) Stop bit(s), corresponding to a binary 1.

5.2.2.2 The time between the stop bit of one character and the start bit of the next character may be of any duration. The data interchange circuit is in the marking condition between characters.

5.2.2.3 Even parity corresponds to a parity bit chosen in such a way that there are an even number of ONE bits in the sequence of data bits and parity bit. Odd parity corresponds to an odd number of ONE bits when formed in the same way.

5.2.2.4 All devices must be capable of sending and receiving characters consisting of one start bit, eight data bits, no parity bit, and one stop bit.

5.2.2.5 The default character structure consists of one start bit, eight data bits, no parity bit, and one stop bit. Eight-data-bit character sets are allowed but not specified by this standard. Other character structures can be used for specialized applications, for example, seven data bits, odd, even, mark or space parity, or two stop bits.

©*Clinical and Laboratory Standards Institute. All rights reserved.*

5.2.2.6 The character bit sequencing, structure, and parity sense definitions conform to ANSI standards X3.15-1976 and X3.16-1976.[12,13]

5.2.3 Speed

5.2.3.1 The data transmission rate for instruments shall be at least one of these baud rates: 1200, 2400, 4800, or 9600 baud. The preferred rate is 9600 baud and should be the default setting of the instrument when more than one baud rate is available. The computer system must have the capability for all four baud rates.

5.2.3.2 Devices may optionally have the capability for other baud rates, such as 300, 19 200, and 38 400 baud for use in specialized applications.

5.2.4 Interface Connections

5.2.4.1 The conforming connection specified here defines the point of interconnection between the domain of the instrument and domain of the computer system. (See Figures 1 and 2.) Within the domain of either device, any appropriate connection system may be used, preferably with suitable cable locking hardware.

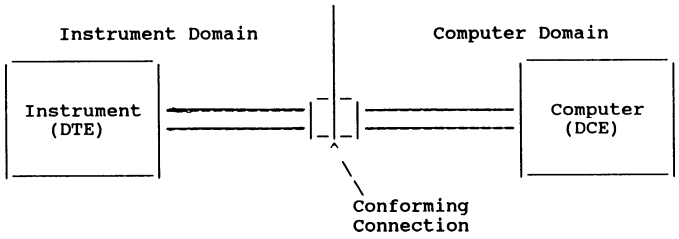

Figure 1. Connector Strategy for Instrument Computer Connection—Cable Mounted

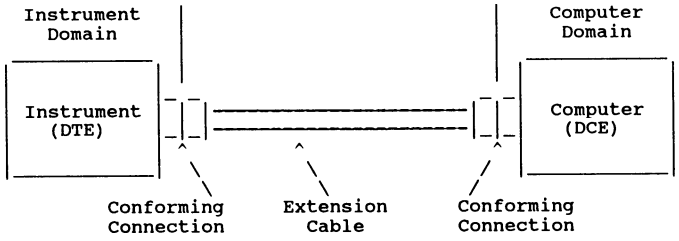

Figure 2. Connector Strategy for Instrument Computer Connections—Chassis Mounted

5.2.4.2 The conforming connection utilizes a 25-position connector. The connector contact assignments are listed in Table 1. Connector contacts not listed are unused. The connector contact assignments conform to the EIA-232-D-1986 standard for the circuits that are used.[11]

Table 1. Connector Contact Assignments for RS 232 D Serial Binary Data Exchange

Contact No.	EIA Circuit	Description	Direction	
			Instrument	Computer
1	...	Shield	...	No Connection
2	BA	Transmitted Data	Output	Input
3	BB	Received Data	Input	Output
7	AB	Signal Ground	...	...

©*Clinical and Laboratory Standards Institute. All rights reserved.*

5.2.4.3 Contact 1 is the shield connection; it connects to the instrument's (the DTE) frame. The shield connection is left open at the computer (the DCE) to avoid ground loops. There will be no connections on any other pins. All other pins will be open circuits.

5.3 Mechanical Characteristics

5.3.1 Connector

5.3.1.1 The conforming connector associated with the instrument is a commercial type DB-25P (subminiature D male) style connector. The conforming connector associated with the computer is a commercial type DB-25S (subminiature D female) style connector. The connector dimensions must correspond to those given in the EIA-232-D-1986 standard.[11]

5.3.1.2 When the conforming connector of the instrument is cable mounted, it shall be configured with a locking device, such as No. 4-40 or M-3 thread female screw locking hardware. When the conforming connector of the computer is cable mounted, it shall be configured with a locking device, such as No. 4-40 or M-3 thread male screw locking hardware. (See Figure 1.)

5.3.1.3 When the conforming connector of either device is chassis mounted, it shall be configured with devices such as No. 4-40 or M-3 thread female screw locking hardware. The mating cable connector shall use devices such as No. 4-40 or M-3 thread male screw locking hardware. (See Figure 2.)

5.3.1.4 When the conforming connector of the instrument is cable mounted and the conforming connector of the computer is chassis mounted, then a change in the cable-mounted locking hardware is necessary.

5.3.2 Cable

Any extension cables to connect the instrument to the computer require a female connector on one end to mate with the instrument and a male connector on the other end to mate with the computer. Detailed requirements of an interconnecting cable are undefined, but good engineering practice should be followed in selecting the cable and connectors. Shielded cable and connectors may be necessary to suppress electromagnetic interface (EMI). Low-capacitance cable may be necessary for long cable lengths or the higher data rates. Appropriate connector-locking hardware should be used at the conforming connectors.

6 Data Link Layer for Serial Binary Data Exchange

6.1 Overview

The data link layer has procedures for link connection and release; delimiting and synchronism; sequential control; error detection; and error recovery.

6.1.1 Link connection and release establish which system sends and which system receives information. Delimiting and synchronism provide for framing of the data and recognition of frames. Sequence control maintains the sequential order of information across the connection. Error detection senses transmission or format errors. Error recovery attempts to recover from detected errors by retransmitting defective frames or returning the link to a neutral state from otherwise unrecoverable errors.

6.1.2 The data link layer uses a character-oriented protocol to send messages between directly connected systems. (See ANSI X3.4-1986. Also, see Appendix B for the coding of the ASCII characters.[14]) Some restrictions are placed on the characters that can appear in the message content.

©*Clinical and Laboratory Standards Institute. All rights reserved.*

6.1.3 The data link mode of operation is one-way transfer of information with alternate supervision. Information flows in one direction at a time. Replies occur after information is sent, never at the same time. It is a simplex stop-and-wait protocol.

6.1.4 At times, the two systems are actively operating to transfer information. The remainder of the time the data link is in a neutral state. See the state diagram in Appendix A.

6.1.5 There are three distinct phases in transferring information between instrument and computer system. In each phase, one system directs the operation and is responsible for continuity of the communication. The three phases ensure the actions of the sender and receiver are coordinated. The three phases are establishment, transfer, and termination.

6.2 Establishment Phase (Link Connection)

6.2.1 The establishment phase determines the direction of information flow and prepares the receiver to accept information.

6.2.2 The sender notifies the receiver that information is available. The receiver responds that it is prepared to receive before information is transmitted.

6.2.3 A system that does not have information to send normally monitors the data link to detect the establishment phase. It acts as a receiver, waiting for the other system.

6.2.4 The system with information available initiates the establishment phase. After the sender determines the data link is in a neutral state, it transmits the **<ENQ>** transmission control character to the intended receiver. The sender will ignore all responses other than **<ACK>, <NAK>,** or **<ENQ>**.

6.2.5 Upon receiving the **<ENQ>**, the receiver prepares to receive information. All other characters are ignored. It replies with the **<ACK>** transmission control character signifying it is ready. With this sequence of events, the establishment phase ends and the transfer phase begins.

6.2.6 A receiver that cannot immediately receive information replies with the **<NAK>** transmission control character. Upon receiving **<NAK>**, the sender must wait at least ten seconds before transmitting another **<ENQ>**.

6.2.7 Systems not having the ability to receive information always respond to an **<ENQ>** by replying with a **<NAK>**. Systems not having the ability to send information never transmit an **<ENQ>**.

6.2.7.1 Contention

Should both systems simultaneously transmit an **<ENQ>**, the data link is in contention. The instrument system has priority to transmit information when contention occurs. Contention is resolved as follows:

(1) Upon receiving a reply of **<ENQ>** to its transmitted **<ENQ>**, the computer system must stop trying to transmit; it must prepare to receive. When the next **<ENQ>** is received, it replies with an **<ACK>** or **<NAK>,** depending on its readiness to receive.

(2) Upon receiving a reply of **<ENQ>** to its transmitted **<ENQ>**, the instrument must wait at least one second before sending another **<ENQ>**.

 ©*Clinical and Laboratory Standards Institute. All rights reserved.*

6.3 Transfer Phase

During the transfer phase, the sender transmits messages to the receiver. The transfer phase continues until all messages are sent.

6.3.1 Frames

Messages are sent in frames; each frame contains a maximum of 64 000 characters (including frame overhead). Messages longer than 64 000 characters are divided between two or more frames.

6.3.1.1 Multiple messages are never combined in a single frame. Every message must begin in a new frame.

6.3.1.2 A frame is one of two types: an intermediate frame or an end frame. Intermediate frames terminate with the characters **<ETB>**, checksum, **<CR>,** and **<LF>**. End frames terminate with the characters **<ETX>**, checksum, **<CR>,** and **<LF>**. A message containing 64 000 characters or less is sent in a single end frame. Longer messages are sent in intermediate frames, with the last part of the message sent in an end frame. The frame structure is illustrated as follows:

<STX> FN text **<ETB>** C1 C2 **<CR>** **<LF>** ← intermediate frame
<STX> FN text **<ETX>** C1 C2 **<CR>** **<LF>** ← end frame

where:

<STX>	=	Start of Text transmission control character
FN	=	single digit Frame Number **0** to **7**
text	=	Data Content of Message
<ETB>	=	End of Transmission Block transmission control character
<ETX>	=	End of Text transmission control character
C1	=	most significant character of checksum **0** to **9** and **A** to **F**
C2	=	least significant character of checksum **0** to **9** and **A** to **F**
<CR>	=	Carriage Return ASCII character
<LF>	=	Line Feed ASCII character

6.3.2 Frame Number

The frame number permits the receiver to distinguish between new and retransmitted frames. It is a single digit sent immediately after the **<STX>** character.

6.3.2.1 The frame number is an ASCII digit ranging from **0** to **7**. The frame number begins at **1** with the first frame of the transfer phase. The frame number is incremented by one for every new frame transmitted. After **7**, the frame number rolls over to **0** and continues in this fashion.

6.3.3 Checksum

The checksum permits the receiver to detect a defective frame. The checksum is encoded as two characters, which are sent after the **<ETB>** or **<ETX>** character. The checksum is computed by adding the binary values of the characters, keeping the least significant eight bits of the result.

©*Clinical and Laboratory Standards Institute. All rights reserved.*

6.3.3.1 The checksum is initialized to zero with the **<STX>** character. The first character used in computing the checksum is the frame number. Each character in the message text is added to the checksum (modulo 256). The computation for the checksum does not include **<STX>**, the checksum characters, or the trailing **<CR>** and **<LF>**.

6.3.3.2 The checksum is an integer represented by eight bits; it can be considered as two groups of four bits. The groups of four bits are converted to the ASCII characters of the hexadecimal representation. The two ASCII characters are transmitted as the checksum, with the most significant character first.

6.3.3.3 For example, a checksum of 122 can be represented as 01111010 in binary or **7A** in hexadecimal. The checksum is transmitted as the ASCII character **7** followed by the character **A**.

6.3.4 Acknowledgments

After a frame is sent, the sender stops transmitting until a reply is received.

6.3.4.1 The receiver replies to each frame. When it is ready to receive the next frame, it transmits one of three replies to acknowledge the last frame. This reply must be transmitted within the timeout period specified in Section 6.5.2.

6.3.4.2 A reply of **<ACK>** signifies the last frame was received successfully, and the receiver is prepared to receive another frame. The sender must increment the frame number and either send a new frame or terminate.

6.3.4.3 A reply of **<NAK>** signifies the last frame was not successfully received, and the receiver is prepared to receive the frame again.

6.3.4.4 A reply of **<EOT>** signifies the last frame was received successfully; the receiver is prepared to receive another frame but requests that the sender stop transmitting. (See the following section on receiver interrupts.)

6.3.5 Receiver Interrupts

The receiver interrupt is a means for the receiver to request the sender to stop transmitting messages as soon as possible.

6.3.5.1 During the transfer phase, if the receiver responds to a frame with an **<EOT>** in place of the usual **<ACK>**, the sender must interpret this reply as a receiver interrupt request. The **<EOT>** is a positive acknowledgment of the end frame, signifies the receiver is prepared to receive next frame, and is a request to the sender to stop transmitting.

6.3.5.2 The sender does not have to stop transmitting after receiving the receiver interrupt request. If the sender chooses to ignore the **<EOT>**, the receiver must re-request the interrupt for the request to remain valid.

6.3.5.3 If the sender chooses to honor the receiver interrupt request, it must first enter the termination phase to return the data link to the neutral state. This gives the receiver an opportunity to enter the establishment phase and become the sender. The original sender must not enter the establishment phase for at least 15 seconds or until the receiver has sent a message and returned the data link to the neutral state.

 ©*Clinical and Laboratory Standards Institute. All rights reserved.*

6.4 Termination Phase (Link Release)

The termination phase returns the data link to the clear or neutral state. The sender notifies the receiver that all messages have been sent.

6.4.1 The sender transmits the **<EOT>** transmission control character and then regards the data link to be in a neutral state. Upon receiving **<EOT>**, the receiver also regards the data link to be in the neutral state.

6.5 Error Recovery

Methods are described that enable both sender and receiver to recover, in an orderly way, from errors in data transmission.

6.5.1 Defective Frames

A receiver checks every frame to guarantee it is valid. A reply of **<NAK>** is transmitted for invalid frames. Upon receiving the **<NAK>**, the sender retransmits the last frame with the same frame number. In this way, transmission errors are detected and automatically corrected.

6.5.1.1 Any characters occurring before the **<STX>** or **<EOT>** or after the end of the block character (the **<ETB>** or **<ETX>**) are ignored by the receiver when checking the frame. A frame should be rejected because:

(1) Any character errors are detected (parity error, framing error, etc.);
(2) The frame checksum does not match the checksum computed on the received frame; or
(3) The frame number is not the same as the last accepted frame or one number higher (modulo 8).

6.5.1.2 Upon receiving a **<NAK>** or any character except an **<ACK>** or **<EOT>** (a **<NAK>** condition), the sender increments a retransmit counter and retransmits the frame. If this counter shows a single frame was sent and not accepted six times, the sender must abort this message by proceeding to the termination phase. An abort should be extremely rare, but it provides a mechanism to escape from a condition where the transfer phase cannot continue.

6.5.2 Timeouts

The sender and receiver both use timers to detect loss of coordination between them. The timers provide a method for recovery if the communication line or the other device fails to respond.

6.5.2.1 During the establishment phase, the sender sets a timer when transmitting the **<ENQ>**. If a reply of an **<ACK>**, **<NAK>**, or **<ENQ>** is not received within 15 seconds, a timeout occurs. After a timeout, the sender enters the termination phase.

6.5.2.2 During the establishment phase, if the computer (as receiver) detects contention, it sets a timer. If an **<ENQ>** is not received within 20 seconds, a timeout occurs. After a timeout, the receiver regards the line to be in the neutral state.

6.5.2.3 During the transfer phase, the sender sets a timer when transmitting the last character of a frame. If a reply is not received within 15 seconds, a timeout occurs. After a timeout, the sender aborts the message transfer by proceeding to the termination phase. As with excessive retransmissions of defective frames, the message must be remembered so it can be completely repeated.

©*Clinical and Laboratory Standards Institute. All rights reserved.*

6.5.2.4 During the transfer phase, the receiver sets a timer when first entering the transfer phase or when replying to a frame. If a frame or **<EOT>** is not received within 30 seconds, a timeout occurs. After a timeout, the receiver discards the last incomplete message and regards the line to be in the neutral state.

6.5.2.5 A receiver must reply to a frame within 15 seconds or the sender will timeout. A receiver can delay its reply for up to 15 seconds to process the frame or to otherwise go into "busy" mode. Longer delays cause the sender to abort the message.

6.5.2.6 Receivers that cannot process messages fast enough to keep up with a sender may cause message buffer overflows in the sender. A sender can normally store at least one complete message. Storage space for more than one outgoing message is desirable but optional.

6.6 Restricted Message Characters

The data link protocol is designed for sending character-based message text. Restrictions are placed on which characters may appear in the message text. The restrictions make it simpler for senders and receivers to recognize replies and frame delimiters. Additional characters are restricted to avoid interfering with software controls for devices such as multiplexers.

6.6.1 A **<LF>** character is not permitted to appear in the message text; it can appear only as the last character of a frame.

6.6.2 None of the ten transmission control characters, the **<LF>** format effector control character, or four device control characters may appear in message text. The restricted characters are: **<SOH>**, **<STX>**, **<ETX>**, **<EOT>**, **<ENQ>**, **<ACK>**, **<DLE>**, **<NAK>**, **<SYN>**, **<ETB>**, **<LF>**, **<DC1>**, **<DC2>**, **<DC3>**, and **<DC4>**.

7 Physical Layer for TCP/IP Data Exchange

7.1 Overview

The mechanical and electrical connection for TCP/IP data transmission between instrument and computer system is described in this section. The topology is not a point-to-point, direct connection between two devices, but utilizes a central hub for device connection.

7.2 Electrical Characteristics

The voltage and impedance levels for the generator and receiver circuits are as specified in the IEEE 802.3 standard.[15]

7.2.1 Signal Levels

7.2.1.1 The signal levels conform to the IEEE 802.3 standard.[15]

7.2.2 Character Structure

7.2.2.1 The method of data transmission is TCP/IP. The order of the bits in a character is:

(1) One start bit, corresponding to a binary 0;
(2) The data bits of the character, least significant bit transmitted first;
(3) Parity bit; and
(4) Stop bit(s), corresponding to a binary 1.

 ©*Clinical and Laboratory Standards Institute. All rights reserved.*

7.2.2.2 The time between the stop bit of one character and the start bit of the next character may be of any duration. The data interchange circuit is in the marking condition between characters.

7.2.2.3 Even parity corresponds to a parity bit chosen in such a way that there are an even number of ONE bits in the sequence of data bits and parity bit. Odd parity corresponds to an odd number of ONE bits when formed in the same way.

7.2.2.4 All devices must be capable of sending and receiving characters consisting of one start bit, eight data bits, no parity bit, and one stop bit.

7.2.2.5 The default character structure consists of one start bit, eight data bits, no parity bit, and one stop bit. Eight-data-bit character sets are allowed but not specified by this standard. Other character structures can be used for specialized applications, for example, seven data bits, odd, even, mark or space parity, or two stop bits.

7.2.2.6 The character bit sequencing, structure, and parity sense definitions conform to ANSI standards X3.15-1976 and X3.16-1976.[12,13]

7.2.3 Speed

7.2.3.1 The data transmission rate for instruments shall conform to IEEE 802.3[15] and operate at least 10 MB/second. A computer system using TCP/IP must have the capability to conform to a minimum speed of 10 MB/second.

7.2.4 Interface Connections

7.2.4.1 The conforming connection specified here defines the point of interconnection between the domain of the instrument and domain of the computer system. (See Figures 3 and 4.) Within the domain of the devices, an RJ45 connection system is used.

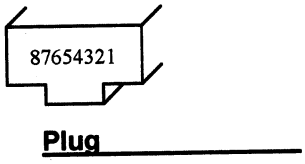

NOTE: Looking at connector end with cable running away from you.

Figure 3. Plug



NOTE: Looking at cavity in the wall.

Figure 4. Jack

7.2.4.2 The conforming connection utilizes an eight-line connector. The connector contact assignments are listed in Table 2. The connector contact assignments conform to the ANSI EIA/TIA 568B standard[16] (also called the AT&T specification).

©*Clinical and Laboratory Standards Institute. All rights reserved.*

Table 2. Connector Contact Assignments

Pin	Color
1	white/orange
2	orange
3	white/green
4	blue
5	white/blue
6	green
7	white/brown
8	brown

7.3 Mechanical Characteristics

7.3.1 Connector

7.3.1.1 The conforming connector associated with the instrument is a commercial type RJ-45F style connector. The conforming connector associated with the computer is a commercial type RJ-45F style connector. The connector dimensions must correspond to those given in the ANSI EIA/TIA 568B standard.[16]

7.3.2 Cable

Category 5 cable as defined by ANSI EIA/TIA 568B[16] is preferred for all connections. In general, no extension cables should be required to connect the instrument to the computer network. Detailed requirements of an interconnecting cable are undefined, but good engineering practice should be followed in selecting the cable and connectors. Low-capacitance cable and shielded connectors may be necessary to suppress electromagnetic interface (EMI). Appropriate connector-locking hardware should be used at the conforming connectors.

8 Data Link Layer for TCP/IP Data Exchange

8.1 Overview

The data link layer has procedures for link connection and release; delimiting and synchronism; sequential control; error detection; and error recovery.

8.1.1 Link connection and release establish which system sends and which system receives information. Delimiting and synchronism provide for framing of the data and recognition of frames. Sequence control maintains the sequential order of information across the connection. Error detection senses transmission or format errors. Error recovery attempts to recover from detected errors by retransmitting defective messages or returning the link to a neutral state from otherwise unrecoverable errors.

8.1.2 The data link layer uses a character-oriented protocol to send messages between directly connected systems. (See ANSI X3.4-1986. Also, see Appendix B for the coding of the ASCII characters.[14]) Some restrictions are placed on the characters that can appear in the message content.

8.1.3 The data link mode of operation is one-way transfer of information with alternate supervision. Information flows in one direction at a time. Replies occur after information is sent, never at the same time. It is a simplex stop-and-wait protocol.

 ©*Clinical and Laboratory Standards Institute. All rights reserved.*

8.1.4 At times, the two systems are actively operating to transfer information. The remainder of the time the data link is in a neutral state. See the state diagram in Appendix A.

8.1.5 There are three distinct phases in transferring information between instrument and computer systems. In each phase, one system directs the operation and is responsible for continuity of the communication. The three phases ensure the actions of the sender and receiver are coordinated. The three phases are establishment, transfer, and termination.

8.2 Establishment Phase (Link Connection)

8.2.1 The establishment phase determines the direction of information flow and prepares the receiver to accept information.

8.2.1.1 The standard framework for TCP/IP network implementation is generally referred to as a "socket" implementation. The normal implementation of a socket-based communication protocol is asymmetric. One end is considered a "server" providing service to the other end, which is considered a "client." Under this client/server paradigm, the "computer system" is defined as the "server," and the "instrument" is defined as the "client." Both ends must initially create sockets and bind their local Internet address to their socket. The computer system, as the server, offers a socket for connection. The instrument (client) must be independently configurable for both socket and IP address (to facilitate use of server-defined socket number and IP address), so it can request a connection to the offered socket.

8.2.2 The sender notifies the receiver that information is available. The receiver responds that it is prepared to receive before information is transmitted.

8.2.3 A system that does not have information to send normally monitors the data link to detect the establishment phase. It acts as a receiver, waiting for the other system.

8.2.4 The system with information available initiates the establishment phase. After the sender determines the data link is in a neutral state, it transmits the **<ENQ>** transmission control character to the intended receiver. The sender will ignore all responses other than **<ACK>**, **<NAK>**, or **<ENQ>**.

8.2.5 Upon receiving the **<ENQ>**, the receiver prepares to receive information. All other characters are ignored. It replies with the **<ACK>** transmission control character signifying it is ready. With this sequence of events, the establishment phase ends and the transfer phase begins.

8.2.6 A receiver that cannot immediately receive information replies with the **<NAK>** transmission control character. Upon receiving **<NAK>**, the sender must wait at least ten seconds before transmitting another **<ENQ>**.

8.2.7 Systems not having the ability to receive information always respond to an **<ENQ>** by replying with a **<NAK>**. Systems not having the ability to send information never transmit an **<ENQ>**.

8.2.7.1 Contention

Should both systems simultaneously transmit an **<ENQ>**, the data link is in contention. The instrument system has priority to transmit information when contention occurs. Contention is resolved as follows:

(1) Upon receiving a reply of **<ENQ>** to its transmitted **<ENQ>**, the computer system must stop trying to transmit; it must prepare to receive. When the next **<ENQ>** is received, it replies with an **<ACK>** or **<NAK>,** depending on its readiness to receive.

©*Clinical and Laboratory Standards Institute. All rights reserved.*

(2) Upon receiving a reply of **<ENQ>** to its transmitted **<ENQ>**, the instrument must wait at least one second before sending another **<ENQ>**.

8.3 Transfer Phase

During the transfer phase, the sender transmits messages to the receiver. The transfer phase continues until all messages are sent.

8.3.1 Frames

Messages are sent in frames; each frame contains a maximum of 64 000 characters (including frame overhead). Messages longer than 63 993 characters are divided between two or more frames.

8.3.1.1 Multiple messages are never combined in a single frame. Every message must begin in a new frame.

8.3.1.2 A frame is one of two types: an intermediate frame or an end frame. Intermediate frames terminate with the characters **<ETB>**, checksum, **<CR>,** and **<LF>**. End frames terminate with the characters **<ETX>**, checksum, **<CR>,** and **<LF>**. A message containing 63 993 characters or less is sent in a single end frame. Longer messages are sent in intermediate frames, with the last part of the message sent in an end frame. The frame structure is illustrated as follows:

<STX> FN text **<ETB>** C1 C2 **<CR>** **<LF>** ← intermediate frame
<STX> FN text **<ETX>** C1 C2 **<CR>** **<LF>** ← end frame

where:

<STX>	=	Start of Text transmission control character
FN	=	single digit Frame Number **0** to **7**
text	=	Data Content of Message
<ETB>	=	End of Transmission Block transmission control character
<ETX>	=	End of Text transmission control character
C1	=	most significant character of checksum **0** to **9** and **A** to **F**
C2	=	least significant character of checksum **0** to **9** and **A** to **F**
<CR>	=	Carriage Return ASCII character
<LF>	=	Line Feed ASCII character

8.3.2 Frame Number

The frame number permits the receiver to distinguish between new and retransmitted frames. It is a single digit sent immediately after the **<STX>** character.

8.3.2.1 The frame number is an ASCII digit ranging from **0** to **7**. The frame number begins at **1** with the first frame of the transfer phase. The frame number is incremented by one for every new frame transmitted. After **7**, the frame number rolls over to **0** and continues in this fashion.

 ©*Clinical and Laboratory Standards Institute. All rights reserved.*

8.3.3 Checksum

The checksum permits the receiver to detect a defective frame. The checksum is encoded as two characters, which are sent after the **<ETB>** or **<ETX>** character. The checksum is computed by adding the binary values of the characters, keeping the least significant eight bits of the result.

8.3.3.1 The checksum is initialized to zero with the **<STX>** character. The first character used in computing the checksum is the frame number. Each character in the message text is added to the checksum (modulo 256). The computation for the checksum does not include **<STX>**, the checksum characters, or the trailing **<CR>** and **<LF>**.

8.3.3.2 The checksum is an integer represented by eight bits; it can be considered as two groups of four bits. The groups of four bits are converted to the ASCII characters of the hexadecimal representation. The two ASCII characters are transmitted as the checksum, with the most significant character first.

8.3.3.3 For example, a checksum of 122 can be represented as 01111010 in binary or **7A** in hexadecimal. The checksum is transmitted as the ASCII character **7** followed by the character **A**.

8.3.4 Acknowledgments

After a frame is sent, the sender stops transmitting until a reply is received.

8.3.4.1 The receiver replies to each frame. When it is ready to receive the next frame, it transmits one of three replies to acknowledge the last frame. This reply must be transmitted within the timeout period specified in Section 8.5.2.

8.3.4.2 A reply of **<ACK>** signifies the last frame was received successfully and the receiver is prepared to receive another frame. The sender must increment the frame number and either send a new frame or terminate.

8.3.4.3 A reply of **<NAK>** signifies the last frame was not successfully received and the receiver is prepared to receive the frame again.

8.3.4.4 A reply of **<EOT>** signifies the last frame was received successfully, the receiver is prepared to receive another frame, but requests that the sender stop transmitting. (See the following section on receiver interrupts.)

8.3.5 Receiver Interrupts

The receiver interrupt is a means for the receiver to request the sender to stop transmitting messages as soon as possible.

8.3.5.1 During the transfer phase, if the receiver responds to a frame with an **<EOT>** in place of the usual **<ACK>**, the sender must interpret this reply as a receiver-interrupt request. The **<EOT>** is a positive acknowledgment of the end frame, signifies the receiver is prepared to receive next frame, and is a request to the sender to stop transmitting.

8.3.5.2 The sender does not have to stop transmitting after receiving the receiver-interrupt request. If the sender chooses to ignore the **<EOT>**, the receiver must re-request the interrupt for the request to remain valid.

©*Clinical and Laboratory Standards Institute. All rights reserved.*

8.3.5.3 If the sender chooses to honor the receiver-interrupt request, it must first enter the termination phase to return the data link to the neutral state. This gives the receiver an opportunity to enter the establishment phase and become the sender. The original sender must not enter the establishment phase for at least 15 seconds or until the receiver has sent a message and returned the data link to the neutral state.

8.4 Termination Phase (Link Release)

The termination phase returns the data link to the clear or neutral state. The sender notifies the receiver that all messages have been sent.

8.4.1 The sender transmits the **<EOT>** transmission control character and then regards the data link to be in a neutral state. Upon receiving **<EOT>**, the receiver also regards the data link to be in the neutral state.

8.5 Error Recovery

Methods are described that enable both sender and receiver to recover, in an orderly way, from errors in data transmission.

8.5.1 Defective Frames

A receiver checks every frame to guarantee it is valid. A reply of **<NAK>** is transmitted for invalid frames. Upon receiving the **<NAK>**, the sender retransmits the last frame with the same frame number. In this way, transmission errors are detected and automatically corrected.

8.5.1.1 Any characters occurring before the **<STX>** or **<EOT>** or after the end of the block character (the **<ETB>** or **<ETX>**) are ignored by the receiver when checking the frame. A frame should be rejected because:

(1) Any character errors are detected (parity error, framing error, etc.);
(2) The frame checksum does not match the checksum computed on the received frame; or
(3) The frame number is not the same as the last accepted frame or one number higher (modulo 8).

8.5.1.2 Upon receiving a **<NAK>** or any character except an **<ACK>** or **<EOT>** (a **<NAK>** condition), the sender increments a retransmit counter and retransmits the frame. If this counter shows a single frame was sent and not accepted six times, the sender must abort this message by proceeding to the termination phase. An abort should be extremely rare, but it provides a mechanism to escape from a condition where the transfer phase cannot continue.

8.5.2 Timeout

The sender and receiver both use timers to detect loss of coordination between them. The timers provide a method for recovery if the communication line or the other device fails to respond.

8.5.2.1 During the establishment phase, the sender sets a timer when transmitting the **<ENQ>**. If a reply of an **<ACK>**, **<NAK>**, or **<ENQ>** is not received within 15 seconds, a timeout occurs. After a timeout, the sender enters the termination phase.

8.5.2.2 During the establishment phase, if the computer (as receiver) detects contention, it sets a timer. If an **<ENQ>** is not received within 20 seconds, a timeout occurs. After a timeout, the receiver regards the line to be in the neutral state.

 ©*Clinical and Laboratory Standards Institute. All rights reserved.*

8.5.2.3 During the transfer phase, the sender sets a timer when transmitting the last character of a frame. If a reply is not received within 15 seconds, a timeout occurs. After a timeout, the sender aborts the message transfer by proceeding to the termination phase. As with excessive retransmissions of defective frames, the message must be remembered so it can be completely repeated.

8.5.2.4 During the transfer phase, the receiver sets a timer when first entering the transfer phase or when replying to a frame. If a frame or **<EOT>** is not received within 30 seconds, a timeout occurs. After a timeout, the receiver discards the last incomplete message and regards the line to be in the neutral state.

8.5.2.5 A receiver must reply to a frame within 15 seconds or the sender will timeout. A receiver can delay its reply for up to 15 seconds to process the frame or to otherwise go into "busy" mode. Longer delays cause the sender to abort the message.

8.5.2.6 Receivers that cannot process messages fast enough to keep up with a sender may cause message buffer overflows in the sender. A sender can normally store at least one complete message. Storage space for more than one outgoing message is desirable but optional.

8.6 Restricted Message Characters

The data link protocol is designed for sending character-based message text. Restrictions are placed on which characters may appear in the message text. The restrictions make it simpler for senders and receivers to recognize replies and frame delimiters. Additional characters are restricted to avoid interfering with software controls for devices such as multiplexers.

8.6.1 A **<LF>** character is not permitted to appear in the message text; it can appear only as the last character of a frame.

8.6.2 None of the ten transmission control characters, the **<LF>** format effector control character, or four device control characters may appear in message text. The restricted characters are: **<SOH>**, **<STX>**, **<ETX>**, **<EOT>**, **<ENQ>**, **<ACK>**, **<DLE>**, **<NAK>**, **<SYN>**, **<ETB>**, **<LF>**, **<DC1>**, **<DC2>**, **<DC3>**, and **<DC4>**.

©*Clinical and Laboratory Standards Institute. All rights reserved.*

References

[1] CLSI/NCCLS. *Specification for Transferring Information Between Clinical Laboratory Instruments and Information Systems; Approved Standard—Second Edition*. CLSI/NCCLS document LIS2-A2. Wayne, PA: NCCLS; 2004.

[2] CLSI/NCCLS. *Standard Guide for Selection of a Clinical Laboratory Information Management System.* CLSI/NCCLS document LIS3-A. Wayne, PA: NCCLS; 2003.

[3] CLSI/NCCLS. *Standard Guide for Documentation of Clinical Laboratory Computer Systems.* CLSI/NCCLS document LIS4-A. Wayne, PA: NCCLS; 2003.

[4] CLSI/NCCLS. *Standard Specification for Transferring Clinical Observations Between Independent Computer Systems*. CLSI/NCCLS document LIS5-A. Wayne, PA: NCCLS; 2003.

[5] CLSI/NCCLS. *Standard Practice for Reporting Reliability of Clinical Laboratory Information Systems.* CLSI/NCCLS document LIS6-A. Wayne, PA: NCCLS; 2003.

[6] CLSI/NCCLS. *Standard Specification for Use of Bar Codes on Specimen Tubes in the Clinical Laboratory*. CLSI/NCCLS document LIS7-A. Wayne, PA: NCCLS; 2003.

[7] CLSI/NCCLS. *Standard Guide for Functional Requirements of Clinical Laboratory Information Management Systems.* CLSI/NCCLS document LIS8-A. Wayne, PA: NCCLS; 2003.

[8] CLSI/NCCLS. *Standard Guide for Coordination of Clinical Laboratory Services within the Electronic Health Record Environment and Networked Architectures*. CLSI/NCCLS document LIS9-A. Wayne, PA: NCCLS; 2003.

[9] ISO. *Information processing systems—Open systems interconnection—Basic reference model.* ISO 7498-1984(E). Geneva: International Organization for Standardization

[10] CLSI/NCCLS. *Laboratory Automation: Communications with Automated Clinical Laboratory Systems, Instruments, Devices, and Information Systems; Approved Standard.* CLSI/NCCLS document AUTO3-A. Wayne, PA: NCCLS; 2000.

[11] EIA. *Interface Between Data Terminal Equipment and Data Circuit-Terminating Equipment Employing Serial Binary Data Interchange*. EIA-232-D-1986. Washington, DC: Electronics Industry Association; 1986.

[12] ANSI. *American National Standard for Bit Sequencing of the American National Standard Code for Information Interchange in Serial-by-Bit Data Transmission.* X3.15-1976. New York, NY: American National Standards Institute; 1976.

[13] ANSI. *American National Standard Character Structure and Character Parity Sense for Serial-by-Bit Data Communication in the American National Standard Code for Information Interchange.* X3.16-1976. New York, NY: American National Standards Institute; 1976.

[14] ANSI. *American National Standard Code for Information Systems—Coded Character Sets—7-Bit American National Standard Code for Information Interchange (7-Bit ASCII).* X3.4-1986. New York, NY: American National Standards Institute; 1986.

[15] IEEE. *Information Technology—Telecommunications and Information Exchange Between Systems—Local and Metropolitan Area Networks—Specific Requirements—Part 3: Carrier Sense Multiple Access With Collision Detection (CSMA/CD) Access Method and Physical Layer Specifications.* IEEE-802.3. Piscataway, NJ: Institute of Electrical and Electronics Engineers; 2000.

[16] ANSI EIA/TIA 568B. *Commercial Building Telecommunications Cabling Standard.* Arlington, VA: Electronic Industries Alliance; 2001.

Additional Reference

INCITS. *Information Technology – ISO 7-bit coded Character Set for Information Interchange [L2]*. INCITS/ISO/IEC 646:1991[R2004]. Washington, DC: InterNational Committee for Information Technology Standards; 2004.

 ©*Clinical and Laboratory Standards Institute. All rights reserved.*

Appendix A. Mandatory Information

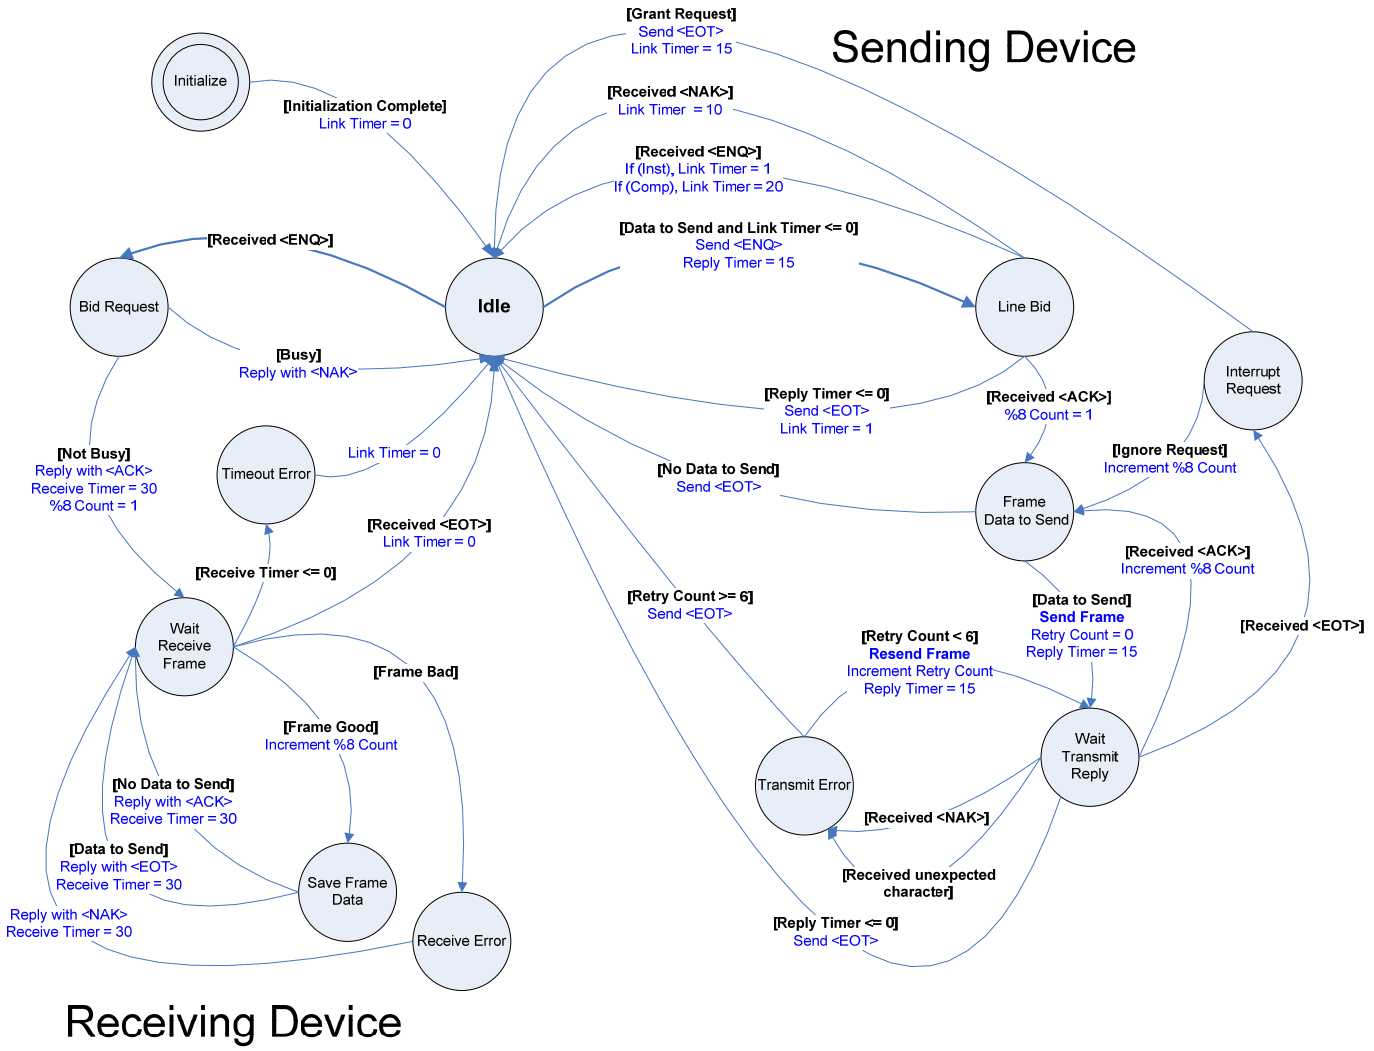

Figure A1. State Diagram

NOTE 1: "%8" represents modulo 8.
NOTE 2: " = " represents assignment of a value. "Timer: = 15" resets the timer to 15 s as used here.

© Clinical and Laboratory Standards Institute. All rights reserved.

Appendix B. Nonmandatory Information

B1. Seven-Bit ASCII Code Charts

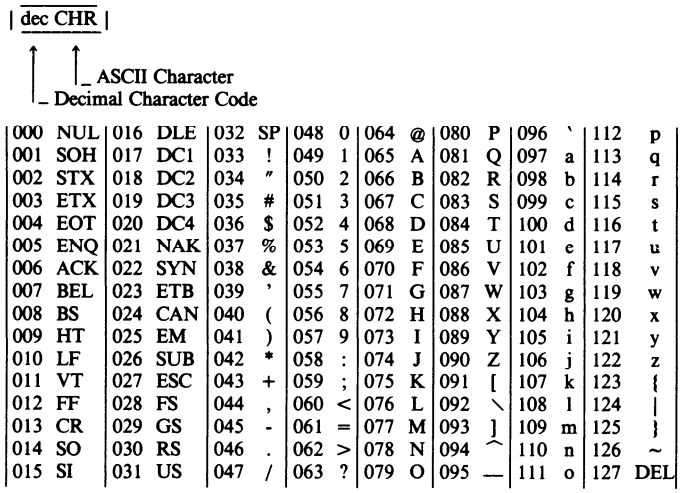

000	NUL	016	DLE	032	SP	048	0	064	@	080	P	096	`	112	p
001	SOH	017	DC1	033	!	049	1	065	A	081	Q	097	a	113	q
002	STX	018	DC2	034	"	050	2	066	B	082	R	098	b	114	r
003	ETX	019	DC3	035	#	051	3	067	C	083	S	099	c	115	s
004	EOT	020	DC4	036	$	052	4	068	D	084	T	100	d	116	t
005	ENQ	021	NAK	037	%	053	5	069	E	085	U	101	e	117	u
006	ACK	022	SYN	038	&	054	6	070	F	086	V	102	f	118	v
007	BEL	023	ETB	039	'	055	7	071	G	087	W	103	g	119	w
008	BS	024	CAN	040	(	056	8	072	H	088	X	104	h	120	x
009	HT	025	EM	041	)	057	9	073	I	089	Y	105	i	121	y
010	LF	026	SUB	042	*	058	:	074	J	090	Z	106	j	122	z
011	VT	027	ESC	043	+	059	;	075	K	091	[	107	k	123	{
012	FF	028	FS	044	,	060	<	076	L	092	\	108	l	124	|
013	CR	029	GS	045	-	061	=	077	M	093	]	109	m	125	}
014	SO	030	RS	046	.	062	>	078	N	094	^	110	n	126	~
015	SI	031	US	047	/	063	?	079	O	095	_	111	o	127	DEL

Figure B1. Decimal Character Code

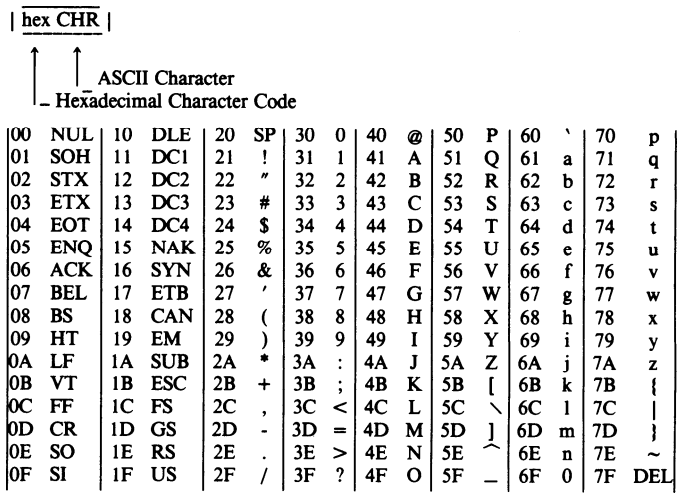

00	NUL	10	DLE	20	SP	30	0	40	@	50	P	60	`	70	p
01	SOH	11	DC1	21	!	31	1	41	A	51	Q	61	a	71	q
02	STX	12	DC2	22	"	32	2	42	B	52	R	62	b	72	r
03	ETX	13	DC3	23	#	33	3	43	C	53	S	63	c	73	s
04	EOT	14	DC4	24	$	34	4	44	D	54	T	64	d	74	t
05	ENQ	15	NAK	25	%	35	5	45	E	55	U	65	e	75	u
06	ACK	16	SYN	26	&	36	6	46	F	56	V	66	f	76	v
07	BEL	17	ETB	27	'	37	7	47	G	57	W	67	g	77	w
08	BS	18	CAN	28	(	38	8	48	H	58	X	68	h	78	x
09	HT	19	EM	29	)	39	9	49	I	59	Y	69	i	79	y
0A	LF	1A	SUB	2A	*	3A	:	4A	J	5A	Z	6A	j	7A	z
0B	VT	1B	ESC	2B	+	3B	;	4B	K	5B	[	6B	k	7B	{
0C	FF	1C	FS	2C	,	3C	<	4C	L	5C	\	6C	l	7C	|
0D	CR	1D	GS	2D	-	3D	=	4D	M	5D	]	6D	m	7D	}
0E	SO	1E	RS	2E	.	3E	>	4E	N	5E	^	6E	n	7E	~
0F	SI	1F	US	2F	/	3F	?	4F	O	5F	_	6F	0	7F	DEL

Figure B2. Hexadecimal Character Code

©Clinical and Laboratory Standards Institute. All rights reserved.

Clinical and Laboratory Standards Institute consensus procedures include an appeals process that is described in detail in Section 8 of the Administrative Procedures. For further information, contact CLSI or visit our website at www.clsi.org.

Summary of Delegate Comments and Area Committee Responses

LIS01-A2: *Specification for Low-Level Protocol to Transfer Messages Between Clinical Laboratory Instruments and Computer Systems; Approved Standard—Second Edition*

General

1. This is a review document of the RS-232 interface, which is rarely used now. Most laboratory equipment comes as an integrated system with simple interfacing software.

- **There are still IVD, middleware, and LIS vendors that make use of this specification for interfaces to legacy and new IVD instruments. There are current IVD vendors that still support RS-232 connectivity to their instruments. Often, this native RS-232 interface may be connected by a very short cable to a device server, either single or multiple ports, but the native instrument datastream is RS-232. The specification still supports these devices.**

2. The College of American Pathologists recommends that the document drafters might want to consider adding commentary about wireless communications possibilities, as the document assumes wired connections.

- **See the response to comment 7 below.**

3. The document describes Ethernet with TCP/IP as an alternative choice for serial communication. The CLIMS shall be TCP/IP-server, the analyzer TCP/IP-client. There are analyzers out in the field that offer ASTM-communication by TCP/IP, but can only play the TCP/IP-server. There is a need for the CLSI standard to permit analyzers as TCP/IP-servers. This behavior is not wrong because analyzers are servers for diagnostic measurements, too. It is also reasonable for the CLIMS to reorganize the analyzer connection after reboot or network shutdown.

- **There are advantages to having the CLIMS assigned the server role. Logically a client-server approach implies one server and many clients, which is true for the case of one CLIMS and multiple instruments. Assigning the instrument the role of client puts control of the initiation and maintenance of the TCP/IP session in the hands of what is presumably the less powerful system. Also, the configuration of the network environment can be simpler if only one server must be identified on the network (the CLIMS), rather than multiple servers if each analyzer were a server. In addition, having the analyzer assigned as the client provides a level of protection for the analyzer, as it must initiate communication rather than receive an unsolicited connection. Finally, if the analyzer is protected by a component such as a firewall, the component would need to be configured to allow the inbound traffic if the analyzer is the server. Configuration is not necessary if the analyzer initiates the communication as a client. This is addressed in Section 8.2.1.1.**

4. Most of the document describes the connectivity hardware. In fact, this hardware is described in other standards very well. If LIS01-A2 would refer to these hardware standards without reproducing, then it is updated automatically after hardware improvements. For example, there is described a 25-pin DB-25 S/P connector, but all modern analyzers are fitted with the newer 9-pin connectors. There is a need for 9-pin connectors to be permitted by the standard.

- **The reviewer makes a good point, but one of the goals for this standard was to maintain compatibility with the previous version. See the response to comment 7 below.**

5. The new standard increases the possible frame length from 255 up to 64 000 characters. This is advantageous for the developer because intermediate frames become no longer necessary, but there is a danger. A 2-digit

©*Clinical and Laboratory Standards Institute. All rights reserved.*

checksum cannot hedge 64 000 bytes in case of serial communication. In case of TCP/IP communication, the frame length can be unlimited without danger and even the checksum is obsolete. I think 64 000 is a bad compromise between 256 and infinity, and there is a need for a frame length reduction in case of serial communication.

- **See Sections 4.4 and 4.4.1, which address the reviewer's comments concerning large frame sizes and restricting their use to TCP/IP communication.**

6. In case of TCP/IP communication, frame length limitations and checksums are obsolete; but compatibility with serial communication requires ability of processing checksums and intermediate frames, so the checksum shall be an optional parameter.

- **As noted by the reviewer, the checksum is no longer required for TCP/IP communication. However, the structure of the frame was not modified for TCP/IP communication in order to maintain complete compatibility with legacy RS-232 interfaces. Compatibility and simplification of frame structure argues against allowing for multiple possible frame structures, and support for an optional checksum parameter introduces opportunities for error based on multiple options. Because the calculation of the checksum is required for serial modes, it introduces no new effort and minimal communication overhead to the standard.**

7. Since the document has been updated to include TCP/IP communication, would it also be possible to include a small section on other communication technologies, such as virtual COM ports over USB, high speed USB, and firewire (IEEE 1394)?

- **Because of the nature of the typical laboratory environment, where a central LIS is connected to multiple instruments located at various locations, it is expected the majority of connections will be RS-232 or TCP/IP. The use of virtual COM ports, through the use of devices such as terminal servers, can be implemented in a manner that is transparent to this specification. Likewise, a wireless implementation could be transparent depending on the implementation. This revision was intended to clarify the existing standards, and the implementation of other technologies is beyond the scope of this effort.**

- **For clarification, Section 4.5 has been added: "Although this specification addresses serial communication using a 25-pin connector and TCP/IP communication, it can be adapted to other standard communication approaches such as a 9-pin serial connector, wireless, high speed USB, and firewire. The physical layer specifications for other approaches must be agreed upon outside the context of this standard. Adaptation to 9-pin, USB, etc. is standard, and can be accomplished in a manner transparent to the specification."**

Table of Contents

8. The proposed Table of Contents is less detailed than it was in the first edition. An original construction of the table was more convenient for users. Preserve the original format of the table (from the first edition).

- **Although less detailed, the Table of Contents is consistent with other CLSI documents (such as LIS2-A2). The structure of the Table of Contents should be consistent across all CLSI documents, and questions about the acceptability/usability of that structure should take place at a higher level than this document.**

Section 3, Terminology

9. It would be helpful for users to see additional terms that were frequently used in a text. Add descriptions for the following terms: stop bit, parity bit, neutral stage, checksum, instrument domain, and computer domain.

- **There are other terms that are not specifically defined in the terminology section, such as TCP/IP. The specification does reference other standards that provide definitions for most terms not listed in the terminology section. The terms used are common to the communications industry and could reasonably be expected to be understood by a reader/user of this standard, or can be understood by reviewing the referenced standards.**

©*Clinical and Laboratory Standards Institute. All rights reserved.*

Section 5.2.3.1

10. The data transmission rate for instruments shall be at least one of these baud rates: 1200, 2400, 4800, or 9600 baud. The preferred rate is 9600 baud, and should be the default setting of the instrument when more than one baud rate is available. The computer system must have the capability for all four baud rates.

    Is it still necessary that when faster baud rates are available (ie, 57 600) that the default setting of the instrument be 9600?

    Is it still true that instruments must support 1200, 2400, 4800, or 9600? And if so, is this meant to ensure compatibility with older computer systems?

    Note: Since the document has been updated to include TCP/IP data exchange, the TCP/IP characteristics specify speed in terms of a "minimum" such as "at least 10MB/sec" vs stating that systems "must support 10MB/sec."

- **The reviewer makes a good point, but legacy compatibility is an important component of the standard. In order to maintain compatibility with existing implementations, it is best to leave the default value at 9600. Note that the wording does not preclude use of faster transmission rates when possible, but rather requires compatibility to slower computer systems to prevent incompatibilities.**

- **"Minimum" was used so as not to exclude other speeds such as 100MB/sec.**

Section 5.2.4.2

11. The conforming connection utilizes a 25-position connector. The connector contact assignments are listed in Table 1. Connector contacts not listed are unused. The connector contact assignments conform to the EIA-232-D-1986 standard for the circuits that are used.

    Is it still a requirement that the conforming interface connection on laboratory instruments utilize a 25-position connector? Considering only four pins are used, and the industry focus on making instruments more compact, a 9-pin connection or possibly a USB type connection would be more appropriate depending on the device. In many cases where serial communication is required, more and more users are running serial-to-Ethernet convertors, or serial-to-USB convertors to attach to systems/networks.

- **See the response to comment 7 above.**

Sections 6.3.1.2 and 8.3.1.2

12. These sections include the same table of frame codes. Include ALL frame code in one comprehensive table that should be added to one of appendixes; exclude tables of frame codes from the body of the standard.

- **The frame layout was included in the original ASTM standard body, as well as the previous CLSI version. The frame layout is included where it might be most immediately referenced, making it easier for a reader to reference the frame definition for a specific implementation (RS-232, TCP/IP). Having to go to an appendix and then back to the body of the document detracts from usability.**

Section 8.2.1.1

13. It might be preferred that the instrument is designated as the server and the computer system is identified as the client. The rationale is that if one has to reboot the computer system for some reason, and it is designated as the "server," all instruments that are connected to it will need to reconnect to that computer system. If the instruments are "servers," they are not affected when the computer system is rebooted.

- **See the discussion and response to comment 3 above.**

©*Clinical and Laboratory Standards Institute. All rights reserved.*

The Quality Management System Approach

Clinical and Laboratory Standards Institute (CLSI) subscribes to a quality management system approach in the development of standards and guidelines, which facilitates project management; defines a document structure via a template; and provides a process to identify needed documents. The approach is based on the model presented in the most current edition of CLSI/NCCLS document HS1—*A Quality Management System Model for Health Care.* The quality management system approach applies a core set of "quality system essentials" (QSEs), basic to any organization, to all operations in any health care service's path of workflow (ie, operational aspects that define how a particular product or service is provided). The QSEs provide the framework for delivery of any type of product or service, serving as a manager's guide. The QSEs are:

Documents & Records	Equipment	Information Management	Process Improvement
Organization	Purchasing & Inventory	Occurrence Management	Customer Service
Personnel	Process Control	Assessments—External & Internal	Facilities & Safety

LIS01-A2 addresses the QSEs indicated by an "X." For a description of the other documents listed in the grid, please refer to the Related CLSI Reference Materials section on the following page.

Documents & Records	Organization	Personnel	Equipment	Purchasing & Inventory	Process Control	Information Management	Occurrence Management	Assessments—External & Internal	Process Improvement	Customer Service	Facilities & Safety
					X AUTO3 LIS2	X AUTO3 LIS2					

Adapted from CLSI/NCCLS document HS1—*A Quality Management System Model for Health Care.*

Path of Workflow

A path of workflow is the description of the necessary steps to deliver the particular product or service that the organization or entity provides. For example, CLSI/NCCLS document GP26—*Application of a Quality Management System Model for Laboratory Services* defines a clinical laboratory path of workflow, which consists of three sequential processes: preexamination, examination, and postexamination. All clinical laboratories follow these processes to deliver the laboratory's services, namely quality laboratory information.

LIS01-A2 addresses the clinical laboratory path of workflow steps indicated by an "X." For a description of the other documents listed in the grid, please refer to the Related CLSI Reference Materials section on the following page.

Preexamination				**Examination**			**Postexamination**	
Examination ordering	Sample collection	Sample transport	Sample receipt/processing	Examination	Results review and follow-up	Interpretation	Results reporting and archiving	Sample management
							X AUTO3 LIS2	

Adapted from CLSI/NCCLS document HS1—*A Quality Management System Model for Health Care.*

©*Clinical and Laboratory Standards Institute. All rights reserved.*

Related CLSI Reference Materials*

AUTO3-A **Laboratory Automation: Communications with Automated Clinical Laboratory Systems, Instruments, Devices, and Information Systems; Approved Standard (2000).** This document provides standards to facilitate accurate and timely electronic exchange of data and information between the automated laboratory elements.

LIS2-A2 **Specification for Transferring Information Between Clinical Laboratory Instruments and Information Systems; Approved Standard—Second Edition (2004).** This document covers the two-way digital transmission of remote requests and results between clinical laboratory instruments and information systems.

* Proposed-level documents are being advanced through the Clinical and Laboratory Standards Institute consensus process; therefore, readers should refer to the most current editions.

©*Clinical and Laboratory Standards Institute. All rights reserved.*

Active Membership
(as of 1 April 2008)

Sustaining Members

Abbott
American Association for Clinical Chemistry
AstraZeneca Pharmaceuticals
Bayer Corporation
BD
Beckman Coulter, Inc.
bioMérieux, Inc.
CLMA
College of American Pathologists
GlaxoSmithKline
Ortho-Clinical Diagnostics, Inc.
Pfizer Inc
Roche Diagnostics, Inc.

Professional Members

American Academy of Family Physicians
American Association for Clinical Chemistry
American Association for Laboratory Accreditation
American Association for Respiratory Care
American Chemical Society
American College of Medical Genetics
American Medical Technologists
American Society for Clinical Laboratory Science
American Society for Microbiology
American Type Culture Collection
ASCP
Associazione Microbiologi Clinici Italiani (AMCLI)
Canadian Society for Medical Laboratory Science
COLA
College of American Pathologists
College of Medical Laboratory Technologists of Ontario
College of Physicians and Surgeons of Saskatchewan
Elkin Simson Consulting Services
ESCMID
Family Health International
Hong Kong Accreditation Service Innovation and Technology Commission
International Federation of Biomedical Laboratory Science
International Federation of Clinical Chemistry
Italian Society of Clinical Biochemistry and Clinical Molecular Biology
JCCLS
The Joint Commission
National Society for Histotechnology, Inc.
Ontario Medical Association Quality Management Program-Laboratory Service
RCPA Quality Assurance Programs PTY Limited
Serbian Society of Microbiology
SIMeL
Sociedad Espanola de Bioquimica Clinica y Patologia Molecular
Sociedade Brasileira de Analises Clinicas
Sociedade Brasileira de Patologia Clinica
Turkish Society of Microbiology
Washington G2 Reports
World Health Organization

Government Members

Armed Forces Institute of Pathology
Association of Public Health Laboratories
BC Centre for Disease Control
Centers for Disease Control and Prevention
Centers for Disease Control and Prevention – Namibia
Centers for Disease Control and Prevention – Nigeria
Centers for Disease Control and Prevention – Tanzania
Centers for Medicare & Medicaid Services
Centers for Medicare & Medicaid Services/CLIA Program
Chinese Committee for Clinical Laboratory Standards
Department of Veterans Affairs
DFS/CLIA Certification
FDA Center for Biologics Evaluation and Research
FDA Center for Devices and Radiological Health
FDA Center for Veterinary Medicine
Health Canada
Massachusetts Department of Public Health Laboratories
Ministry of Health and Social Welfare – Tanzania
National Center of Infectious and Parasitic Diseases (Bulgaria)
National Health Laboratory Service (South Africa)
National Institute of Standards and Technology
National Pathology Accreditation Advisory Council (Australia)
New York State Department of Health
Ontario Ministry of Health
Pennsylvania Dept. of Health
Saskatchewan Health-Provincial Laboratory
Scientific Institute of Public Health
University of Iowa, Hygienic Lab

Industry Members

3M Medical Division
AB Biodisk
Abbott
Abbott Diabetes Care
Abbott Molecular Inc.
Abbott Point of Care Inc.
Access Genetics
Acupath
AdvaMed
Advancis Pharmaceutical Corporation
Advantage Bio Consultants, Inc.
Affymetrix, Inc. (Santa Clara, CA)
Affymetrix, Inc. (W. Sacramento, CA)
Agilent Technologies/Molecular Diagnostics
Ammirati Regulatory Consulting
Anapharm, Inc.
Anna Longwell, PC
Aptium Oncology
Arpida Ltd.
A/S Rosco
Associate Regional & University Pathologists
Astellas Pharma
AstraZeneca Pharmaceuticals
Aviir, Inc.
Axis-Shield PoC AS
Bayer Corporation – West Haven, CT
Bayer HealthCare, LLC, Diagnostics Div. – Elkhart, IN
BD
BD Biosciences – San Jose, CA
BD Diagnostic Systems
BD Vacutainer Systems
Beckman Coulter, Inc.
Beth Goldstein Consultant (PA)
Bioanalyse, Ltd.
Bio-Development S.r.l.
Biomedia Laboratories SDN BHD
bioMérieux, Inc. (MO)
bioMérieux, Inc. (NC)
Bio-Rad Laboratories, Inc. – France
Bio-Rad Laboratories, Inc. – Irvine, CA
Bio-Rad Laboratories, Inc. – Plano, TX
Blaine Healthcare Associates, Inc.
Braun Biosystems, Inc.
Canon U.S. Life Sciences, Inc.
Cempra Pharmaceuticals, Inc.
Center for Measurement Standards/ITRI
Centers for Disease Control and Prevention
Central States Research Centre, Inc.
Cepheid
Chen & Chen, LLC (IQUUM)
The Clinical Microbiology Institute
Comprehensive Cytometric Consulting
Control Lab
Copan Diagnostics Inc.
Cosmetic Ingredient Review
Cubist Pharmaceuticals
Cumbre Inc.
Dade Behring Marburg GmbH – A Siemens Company
Dahl-Chase Pathology Associates PA
David G. Rhoads Associates, Inc.
Diagnostic Products Corporation
Diagnostica Stago
Docro, Inc.
DX Tech
Eiken Chemical Company, Ltd.
Elanco Animal Health
Emisphere Technologies, Inc.
Eurofins Medinet
Fio
Focus Diagnostics
Future Diagnostics B.V.
Genomic Health, Inc.
Gen-Probe
Genzyme Diagnostics
GlaxoSmithKline
GlucoTec, Inc.
GR Micro LTD
Greiner Bio-One Inc.
Habig Regulatory Consulting
HistoGenex N.V.
Icon Laboratories, Inc.
Immunicon Corporation
Indiana State Department of Health
Instrumentation Laboratory
Japan Assn. of Clinical Reagents Industries
Joanneum Research Forschungsgesellschaft mbH
Johnson & Johnson Pharmaceutical Research and Development, L.L.C.
Kaiser Permanente
K.C.J. Enterprises
Krouwer Consulting
Laboratory Specialists, Inc.
LifeScan, Inc. (a Johnson & Johnson Company)
LipoScience
Maine Standards Company, LLC
Medical Device Consultants, Inc.
Merck & Company, Inc.
Micromyx, LLC
MicroPhage
Monogen, Inc.
MultiPhase Solutions, Inc.
Nanogen
Nanogen, Point-of-Care Diagnostics Div.
Nanosphere, Inc.
Nihon Koden Corporation
Nissui Pharmaceutical Co., Ltd.
NJK & Associates, Inc.
NorDx – Scarborough Campus
NovaBiotics (Aberdeen, UK)
Novartis Institutes for Biomedical Research
Nucryst Pharmaceuticals
Olympus America, Inc.
Opti Scan Bio Medical Assoc.
Optimer Pharmaceuticals, Inc.
Orion Genomics, LLC
Ortho-Clinical Diagnostics, Inc. (Rochester, NY)
Ortho-McNeil, Inc.
Oxonica (UK)
Panaceapharma Pharmaceuticals
Paratek Pharmaceuticals, Inc.
PathCare
Pathwork Diagnostics
Pfizer Animal Health
Pfizer Inc
Phadia AB
PlaCor, Inc
Powers Consulting Services
PPD
ProSource Consulting, Inc.
QSE Consulting
Qualtek Clinical Laboratories
Quest Diagnostics, Incorporated
Radiometer America, Inc.
RCC CIDA S. A.
Replidyne
Rib-X Pharmaceuticals
Roche Diagnostics GmbH
Roche Diagnostics, Inc.
Roche Diagnostics Ltd
Roche Diagnostics Shanghai Ltd.
Roche Molecular Systems
SAIC Frederick Inc. NCI-Frederick Cancer Research & Development Center
Sanofi Pasteur
Sarstedt, Inc.
Schering Corporation
Sequenom, Inc.
Siemens Healthcare Diagnostics
Siemens Medical Solutions Diagnostics (CA)
Siemens Medical Solutions Diagnostics (DE)
Siemens Medical Solutions Diagnostics (NY)
Specialty Ranbaxy Ltd
Sphere Medical Holding Limited
State of Alabama
Stirling Medical Innovations
Streck Laboratories, Inc.
Sysmex America, Inc. (Mundelein, IL)
Sysmex Corporation (Japan)
Targanta Therapeutics, Inc
Tethys Bioscience, Inc.
TheraDoc
Therapeutic Monitoring Services, LLC
Theravance Inc.
Third Wave Technologies, Inc.
Thrombodyne, Inc.
ThromboVision, Inc.
Transasia Bio-Medicals Limited
Trek Diagnostic Systems
Upside Endeavors, LLC
Vital Diagnostics S.r.l.
Watin-Biolife Diagnostics and Medicals
Wellstat Diagnostics, LLC
Wyeth Research
XDX, Inc.
YD Consultant
ZIUR Ltd.

Trade Associations

AdvaMed
Japan Association of Clinical Reagents Industries (Tokyo, Japan)

Associate Active Members

3rd Medical Group (AK)
5th Medical Group/SGSL (ND)
22 MDSS (KS)
36th Medical Group/SGSL (Guam)
48th Medical Group/MDSS (APO, AE)
55th Medical Group/SGSAL (NE)
59th MDW/859th MDTS/MTL Wilford Hall Medical Center (TX)
Academisch Ziekenhuis-VUB
Acadiana Medical Labs, Ltd
ACL Laboratories (IL)
Adams County Hospital (OH)
Air Force Institute for Operational Health (TX)
Akron's Children's Hospital (OH)
Alameda County Medical Center
Albany Medical Center Hospital (NY)
Albemarle Hospital (NC)
Alfred I. du Pont Hospital for Children
All Children's Hospital (FL)
Allegheny General Hospital (PA)
Alpena General Hospital (MI)
Alta Bates Summit Medical Center (CA)
American University of Beirut Medical Center (NJ)
Anne Arundel Medical Center (MD)
Antelope Valley Hospital District (CA)
Arkansas Children's Hospital (AR)
Arkansas Dept of Health Public Health Laboratory (AR)
Arkansas Methodist Medical Center (AR)
Asan Medical Center (Seoul)
Asante Health System (OR)
Asiri Group of Hospitals Ltd.
Asociacion Espanola Primera de Socorros Mutuos (Uruguay)
Aspirus Wausau Hospital (WI)
Atlantic City Medical Center (NJ)
Atlantic Health Sciences Corp.
Auburn Regional Medical Center (WA)
Augusta Medical Center (VA)
Aultman Hospital (OH)
Avera McKennan (SD)
Az Sint-Jan
Azienda Ospedale Di Lecco (Italy)
Baffin Regional Hospital (Canada)
Baptist Hospital for Women (TN)
Baptist Hospital of Miami (FL)
Bassett Army Community Hospital (AK)
Baton Rouge General (LA)
Baxter Regional Medical Center (AR)
Bay Regional Medical Center (MI)
BayCare Health System (FL)
Baylor Health Care System (TX)
Bayou Pathology, APMC (LA)
Baystate Medical Center (MA)
B.B.A.G. Ve U. AS., Duzen Laboratories (Turkey)
Beebe Medical Center (DE)
Belfast HSS Trust

Beloit Memorial Hospital (WI)
Ben Taub General Hospital (TX)
The Bermuda Hospitals Board
Bonnyville Health Center (Canada)
Boston Medical Center (MA)
Boulder Community Hospital (CO)
Brantford General Hospital (Canada)
Bridgeport Hospital (CT)
Bronson Methodist Hospital (MI)
Broward General Medical Center (FL)
Calgary Laboratory Services (Calgary, AB, Canada)
California Pacific Medical Center (CA)
Cambridge Health Alliance (MA)
Camden Clark Memorial Hospital (WV)
Canadian Science Center for Human and Animal Health (Canada)
Cape Breton Healthcare Complex (Canada)
Cape Cod Hospital (MA)
Cape Fear Valley Medical Center Laboratory (NC)
Capital Health/QE II Health Sciences Centre (Nova Scotia)
Capital Health - Regional Laboratory Services (Canada)
Capital Health System Mercer Campus (NJ)
Carilion Labs Charlotte
Carpermor S.A. de C.V. (Mexico)
Catholic Health Initiatives (KY)
Cavan General Hospital (Ireland)
CDC/HIV (APO, AP)
Cedars-Sinai Medical Center (CA)
Central Baptist Hospital (KY)
Central Kansas Medical Center (KS)
Central Texas Veterans Health Care System (TX)
Centralized Laboratory Services (NY)
Centre Hospitalier Anna-Laberge (Canada)
Centura – Villa Pueblo (CO)
Chaleur Regional Hospital (Canada)
Chang Gung Memorial Hospital (Taiwan)
Changhua Christian Hospital (Taiwan)
The Charlotte Hungerford Hospital (CT)
Chatham - Kent Health Alliance (Canada)
Chesapeake General Hospital (VA)
Chester County Hospital (PA)
Children's Healthcare of Atlanta (GA)
The Children's Hospital (CO)
Children's Hospital (OH)
Children's Hospital and Medical Center (WA)
Children's Hospital & Research Center at Oakland (CA)
Children's Hospital Medical Center (OH)
Children's Hospital of Philadelphia (PA)
Children's Hospitals and Clinics (MN)
Children's Medical Center (OH)
Children's Medical Center (TX)
Children's Memorial Hospital (IL)
The Children's Mercy Hospital (MO)
Childrens Hosp. – Kings Daughters (VA)
Childrens Hospital Los Angeles (CA)
Childrens Hospital of Wisconsin (WI)
Chilton Memorial Hospital (NJ)
Christiana Care Health Services (DE)
Christus St. John Hospital (TX)
CHU Sainte – Justine (Quebec)
City of Hope National Medical Center (CA)
Clarian Health – Clarian Pathology Laboratory (IN)
Cleveland Clinic Health System Eastern Region (OH)
Clinical Labs of Hawaii (HI)
CLSI Laboratories, Univ. Pittsburgh Med. Ctr. (PA)
Colchester East Hants Health Authority (Canada)
Commonwealth of Virginia (DCLS) (VA)
Community Hospital (IN)
The Community Hospital (OH)
Community Hospital of the Monterey Peninsula (CA)
Community Medical Center (NJ)
Community Memorial Hospital (WI)
Consultants Laboratory of WI LLC (WI)
Contra Costa Regional Medical Center (CA)
Cook Children's Medical Center (TX)
Cork University Hospital (Ireland)
Corpus Christi Medical Center (TX)
Covance CLS (IN)
Covance Evansville (IN)
The Credit Valley Hospital (Canada)
Creighton Medical Laboratories (NE)
Creighton University Medical Center (NE)
Crozer-Chester Medical Center (PA)
Darwin Library NT Territory Health Services (Australia)
David Grant Medical Center (CA)
Daviess Community Hospital (IN)
Deaconess Hospital Laboratory (IN)
Deaconess Medical Center (WA)
Dean Medical Center (WI)
DeWitt Healthcare Network (USA Meddac) (VA)
DHHS NC State Lab of Public Health (NC)
Diagnostic Laboratory Services, Inc. (HI)
Diagnostic Services of Manitoba (Canada)
Diagnósticos da América S/A (Sao Paulo)
DIANON Systems/Lab Corp. (OK)
Diaz Gill-Medicina Laboratorial S.A.
Dimensions Healthcare System (MD)
Dr. Erfan & Bagedo General Hospital (Saudi Arabia)
Dr. Everette Chalmers Regional Hospital (NB)
DRAKE Center (OH)
Driscoll Children's Hospital (TX)
DSI of Bucks County (PA)
DUHS Clinical Laboratories (NC)
Dundy County Hospital (NE)
Durham VA Medical Center (NC)
DVA Laboratory Services (FL)
Dwight D. Eisenhower Medical Center (KS)
E. A. Conway Medical Center (LA)
East Central Health (Canada)
East Georgia Regional Medical Center (GA)
Eastern Health Pathology (Australia)
Easton Hospital (PA)
Edward Hospital (IL)
Effingham Hospital (GA)
Eliza Coffee Memorial Hospital (AL)
Emory University Hospital (GA)
Evangelical Community Hospital (PA)
Evans Army Community Hospital (CO)
Exeter Hospital (NH)
Federal Medical Center (MN)
First Health of the Carolinas Moore Regional Hospital (NC)
Flaget Memorial Hospital (KY)
Fletcher Allen Health Care (VT)
Fleury S.A. (Brazil)
Florida Hospital (FL)
Florida Hospital Waterman (FL)
Foote Hospital (MI)
Fort St. John General Hospital (Canada)
Forum Health Northside Medical Center (OH)
Fox Chase Cancer Center (PA)
Frankford Hospital (PA)
Fraser Health Authority Royal Columbian Hospital Site (Canada)
Fresenius Medical Care/Spectra East (NJ)
Fundacio Joan Costa Roma Consorci Sanitari de Terrassa (Spain)
Gamma-Dynacare Laboratories (Canada)
Gamma Dynacare Medical Laboratories (Ontario, Canada)
Garden City Hospital (MI)
Garfield Medical Center (CA)
Geisinger Medical Center (Danville, PA)
Genesis Healthcare System (OH)
George Washington University Hospital (DC)
Ghent University Hospital (Belgium)
Good Samaritan Hospital (OH)
Good Shepherd Medical Center (TX)
Grana S.A. (Mexico)
Grand Strand Reg. Medical Center (SC)
Gundersen Lutheran Medical Center (WI)
Guthrie Clinic Laboratories (PA)
Haga Teaching Hospital (Netherlands)
Hagerstown Medical Laboratory (MD)
Halton Healthcare Services (Canada)
Hamad Medical Corporation (Qatar)
Hamilton Regional Laboratory Medicine Program (Canada)
Hanover General Hospital (PA)
Harford Memorial Hospital (MD)
Harris Methodist Fort Worth (TX)
Health Network Lab (PA)
Health Partners Laboratories Bon Secours Richmond (VA)
Health Sciences Research Institute (Japan)
Health Waikato (New Zealand)
Heartland Health (MO)
Heidelberg Army Hospital (APO, AE)
Helen Hayes Hospital (NY)
Hema-Quebec (Canada)
Hennepin Faculty Association (MN)
Henry Ford Hospital (MI)
Henry M. Jackson Foundation (MD)
Henry Medical Center, Inc. (GA)
Hi-Desert Medical Center (CA)
Hoag Memorial Hospital Presbyterian (CA)
Holy Cross Hospital (MD)
Holy Family Medical Center (WI)
Holy Name Hospital (NJ)
Holy Spirit Hospital (PA)
Hopital Cite de La Sante de Laval (Canada)
Hopital du Haut-Richelieu (Canada)
Hôpital Maisonneuve - Rosemont (Montreal, Canada)
Hôpital Sacré-Coeur de Montreal (Quebec, Canada)
Hopital Santa Cabrini Ospedale (Canada)
Hospital Albert Einstein (Brazil)
Hospital das Clinicas-FMUSP (Brazil)
Hospital de Dirino Espirito Santa (Portugal)
The Hospital for Sick Children (Canada)
Hôtel Dieu Grace Hospital Library (Windsor, ON, Canada)
Hunter Area Pathology Service (Australia)
Imelda Hospital (Belgium)
Indiana University – Chlamydia Laboratory (IN)
Inova Fairfax Hospital (VA)
Institut fur Stand. und Dok. im Med. Lab. (Germany)
Institut National de Santé Publique du Quebec Centre de Doc. – INSPQ (Canada)
Institute Health Laboratories (PR)
Institute of Clinical Pathology and Medical Research (Australia)
Institute of Laboratory Medicine Landspitali Univ. Hospital (Iceland)
Institute of Medical & Veterinary Science (Australia)
Integrated Regional Laboratories South Florida (FL)
International Health Management Associates, Inc. (IL)
Ireland Army Community Hospital (KY)
IWK Health Centre (Canada)
Jackson County Memorial Hospital (OK)
Jackson Health System (FL)
Jackson Purchase Medical Center (KY)
Jacobi Medical Center (NY)
John C. Lincoln Hospital (AZ)
John Muir Medical Center (CA)
John T. Mather Memorial Hospital (NY)
Johns Hopkins Medical Institutions (MD)
Johns Hopkins University (MD)
Johnson City Medical Center (TN)
JPS Health Network (TX)
Kadlec Medical Center (WA)
Kaiser Permanente (CA)
Kaiser Permanente (MD)
Kaiser Permanente (OH)
Kaiser Permanente Medical Care (CA)
Kantonsspital Aarau AG (Switzerland)
Keller Army Community Hospital (NY)
Kenora-Rainy River Reg. Lab. Program (Canada)
King Fahad National Guard Health Affairs King Abdulaziz Medical City (Saudi Arabia)
King Faisal Specialist Hospital (MD)
King Hussein Cancer Center
Kings County Hospital Center (NY)
Kingston General Hospital (Canada)
Lab Medico Santa Luzia LTDA (Brazil)
Labette Health (KS)
Laboratory Alliance of Central New York (NY)
LabPlus Auckland Healthcare Services Limited (New Zealand)
Labway Clinical Laboratory Ltd (China)
Lafayette General Medical Center (LA)
Lakeland Regional Laboratories (MI)
Lakeland Regional Medical Center (FL)
Lancaster General Hospital (PA)
Landstuhl Regional Medical Center
Langley Air Force Base (VA)
LeBonheur Children's Medical Center (TN)
Legacy Laboratory Services (OR)
Lethbridge Regional Hospital (Canada)
Lewis-Gale Medical Center (VA)
L'Hotel-Dieu de Quebec (Quebec, Canada)
Licking Memorial Hospital (OH)
LifeBridge Health Sinai Hospital (MD)
LifeLabs (Canada)
Loma Linda University Medical (CA)
Long Beach Memorial Medical Center (CA)
Los Angeles County Public Health Lab. (CA)
Louisiana Office of Public Health Laboratory (LA)
Louisiana State University Medical Ctr. (LA)
Lourdes Hospital (KY)
Maccabi Medical Care and Health Fund
Madison Parish Hospital (LA)
Mafraq Hospital
Magnolia Regional Health Center (MS)
Main Line Clinical Laboratories, Inc. (PA)
Maricopa Integrated Health System (AZ)
Marquette General Hospital (MI)
Marshfield Clinic (WI)
Martha Jefferson Hospital (VA)
Martin Luther King, Jr. Harbor Hospital (CA)
Martin Memorial Health Systems (FL)
Mary Imogene Bassett Hospital (NY)
Marymount Medical Center (KY)
Massachusetts General Hospital (MA)
Massachusetts General Hospital Division of Laboratory Medicine (MA)
Maxwell Air Force Base (AL)
Mayo Clinic (MN)
Mayo Clinic Scottsdale (AZ)
MDS Metro Laboratory Services (BC, Canada)
Meadows Regional Medical Center (GA)
Mease Countryside Hospital (FL)
Medecin Microbiologiste (Canada)
Medical Center Hospital (TX)
Medical Center of Louisiana at NO-Charity (LA)
Medical Center of McKinney (TX)
Medical Centre Ljubljana (Slovenia)
Medical College of Virginia Hospital (VA)
Medical Specialists (IN)
Medical Univ. of South Carolina (SC)
MediCorp - Mary Washington Hospital (VA)
Memorial Hermann Healthcare System (TX)
Memorial Hospital at Gulfport (MS)
Memorial Hospital Laboratory (CO)
Memorial Medical Center (IL)
Memorial Medical Center (PA)
Memorial Regional Hospital (FL)
Mercy Franciscan Mt. Airy (OH)
Mercy Hospital (ME)
Mercy Medical Center (CO)
Mercy Medical Center (OR)
Methodist Hospital (MN)
Methodist Hospital (TX)
Methodist Hospital Pathology (NE)
MetroHealth Medical Center (OH)
Metropolitan Hospital Center (NY)
Metropolitan Medical Laboratory, PLC (IA)
The Michener Inst. for Applied Health Sciences (Canada)
Middelheim General Hospital
Middletown Regional Hospital (OH)
Mike O'Callaghan Federal Hospital (NV)
Mississippi Baptist Medical Center (MS)
Mississippi Public Health Lab (MS)
Monmouth Medical Center (NJ)
Montefiore Medical Center (NY)
Montreal General Hospital (Quebec)
Morton Plant Hospital (FL)
Mt. Sinai Hospital - New York (NY)
Nassau County Medical Center (NY)
National Cancer Center (S. Korea)
National Cancer Institute (MD)
National Healthcare Group (Singapore)
National Institutes of Health, Clinical Center (MD)
National Naval Medical Center (MD)
National University Hospital Department of Laboratory Medicine (Singapore)
Naval Hospital Great Lakes (IL)
Naval Hospital Oak Harbor (WA)
Naval Medical Center Portsmouth (VA)
NB Department of Health
The Nebraska Medical Center (NE)
New England Baptist Hospital (MA)
New England Fertility Institute (CT)
New Lexington Clinic (KY)
New York City Department of Health and Mental Hygiene (NY)
New York-Presbyterian Hospital (NY)
New York University Medical Center (NY)
Newark Beth Israel Medical Center (NJ)
Newton Memorial Hospital (NJ)
North Bay Hospital (FL)
North Carolina Baptist Hospital (NC)
North Coast Clinical Laboratory, Inc. (OH)
North District Hospital (Hong Kong)
North Mississippi Medical Center (MS)
North Shore-Long Island Jewish Health System Laboratories (NY)
Northeast Pathologists, Inc. (MO)
Northridge Hospital Medical Center (CA)
Northside Hospital (GA)
Northwest Texas Hospital (TX)
Northwestern Memorial Hospital (IL)
Norton Healthcare (KY)
Ochsner Clinic Foundation (LA)
Ohio State University Hospitals (OH)
Onze Lieve Vrouw Ziekenhuis (Belgium)
Ordre Professionel des Technologistes Medicaux du Quebec (Quebec)
Orebro University Hospital

Orlando Regional Healthcare System (FL)
The Ottawa Hospital (Canada)
Our Lady of Lourdes Medical Center (NJ)
Our Lady of Lourdes Reg. Medical Ctr. (LA)
Our Lady of the Way Hospital (KY)
Our Lady's Hospital for Sick Children (Ireland)
Overlake Hospital Medical Center (WA)
Palmetto Health Baptist Laboratory (SC)
Pathologists Associated (IN)
Pathology and Cytology Laboratories, Inc. (KY)
Pathology Associates Medical Laboratories (WA)
Penn State Hershey Medical Center (PA)
Pennsylvania Hospital (PA)
Penrose St. Francis Health Services (CO)
The Permanente Medical Group (CA)
Perry County Memorial Hospital (IN)
Peterborough Regional Health Centre (Canada)
Piedmont Hospital (GA)
Pitt County Memorial Hospital (NC)
Prairie Lakes Hospital (SD)
Presbyterian Hospital of Dallas (TX)
Presbyterian/St. Luke's Medical Center (CO)
Prince County Hospital
Princess Margaret Hospital (Hong Kong)
Providence Alaska Medical Center (AK)
Providence Health Care (Canada)
Providence Medford Medical Center (OR)
Provincial Health Services Authority (Vancouver, BC, Canada)
Provincial Laboratory for Public Health (Edmonton, AB, Canada)
Queen Elizabeth Hospital (Canada)
Queensland Health Pathology Services (Australia)
Quest Diagnostics, Inc
Quest Diagnostics, Inc (San Juan Capistrano, CA)
Quest Diagnostics JV (IN, OH, PA)
Quest Diagnostics Laboratories (WA)
Quincy Hospital (MA)
Rady Children's Hospital San Diego (CA)
Redington-Fairview General Hospital (ME)
Regional Health Authority Four (RHA4) (Canada)
Regions Hospital (MN)
Reid Hospital & Health Care Services (IN)
Renown Regional Medical Center (NV)
Research Medical Center (MO)
Riverside Regional Medical Center (VA)
Riyadh Armed Forces Hospital, Sulaymainia
Robert Wood Johnson University Hospital (NJ)
Roxborough Memorial Hospital (PA)
Royal Victoria Hospital (Canada)
Rush North Shore Medical Center (IL)
SAAD Specialist Hospital (Saudi Arabia)
Sacred Heart Hospital (FL)
Sacred Heart Hospital (WI)
Sahlgrenska Universitetssjukhuset (Sweden)
Saint Elizabeth Regional Medical Center (NE)
Saint Francis Hospital & Medical Center (CT)
Saint Mary's Regional Medical Center (NV)
Saints Memorial Medical Center (MA)
St. Agnes Healthcare (MD)
St. Anthony Hospital (OK)
St. Anthony Hospital Central Laboratory (CO)
St. Anthony's Hospital (FL)
St. Barnabas Medical Center (NJ)
St. Christopher's Hospital for Children (PA)
St. Elizabeth Community Hospital (CA)
St. Francis Hospital (SC)
St. Francis Medical Center (MN)
St. John Hospital and Medical Center (MI)
St. John's Hospital (IL)
St. John's Hospital & Health Ctr. (CA)
St. John's Mercy Medical Center (MO)
St. John's Regional Health Center (MO)
St. Joseph Medical Center (MD)
St. Joseph Mercy – Oakland (MI)
St. Joseph Mercy Hospital (MI)
St. Joseph's Hospital (FL)
St. Joseph's Hospital & Health Center (ND)
St. Joseph's Medical Center (CA)
St. Joseph's Regional Medical Center (NJ)
St. Jude Children's Research Hospital (TN)
St. Louis University Hospital (MO)
St. Luke's Hospital (FL)
St. Luke's Hospital (IA)
St. Luke's Hospital (PA)
St. Margaret Memorial Hospital (PA)
St. Martha's Regional Hospital (Canada)
St. Mary Medical Center (CA)
St. Mary's Health Center (MO)
St Mary's Healthcare (SD)
St. Mary's Medical Center (IN)
St. Michael's Hospital Diagnostic Laboratories & Pathology (Canada)
St. Tammany Parish Hospital (LA)
St. Thomas More Hospital (CO)
Sampson Regional Medical Center (NC)
Samsung Medical Center (Korea)
San Francisco General Hospital-University of California San Francisco (CA)
Sanford USP Medical Center (SD)
SARL Laboratoire Carron (France)
Saudi Aramco Medical (Saudi Arabia)
Scott Air Force Base (IL)
Scott & White Memorial Hospital (TX)
Seoul National University Hospital (Korea)
Seton Medical Center (CA)
Shamokin Area Community Hospital (PA)
Sheik Kalifa Medical City (UAE)
Shore Memorial Hospital (NJ)
Shriners Hospitals for Children (SC)
Singapore General Hospital (Singapore)
SJRMC Plymouth Laboratory (IN)
Sky Lakes Medical Center (OR)
South Bend Medical Foundation (IN)
South County Hospital (RI)
South Dakota State Health Laboratory (SD)
South Miami Hospital (FL)
Southern Health Care Network (Australia)
Southern Maine Medical Center (ME)
Southwest Nova District Health Authority (Canada)
Speare Memorial Hospital (NH)
Spectrum Health - Blodgett Campus (MI)
Stanford Hospital and Clinics (CA)
State of Connecticut Department of Public Health (CT)
State of Hawaii Department of Health (HI)
State of Washington-Public Health Labs (WA)
Steele Memorial Hospital (ID)
Stillwater Medical Center (OK)
Stony Brook University Hospital (NY)
Stormont-Vail Regional Medical Center (KS)
Sudbury Regional Hospital (Canada)
Suncoast Medical Clinic (FL)
Sunnybrook Health Science Center (ON, Canada)
Sunrise Hospital and Medical Center (NV)
Swedish Medical Center (CO)
Sydney South West Pathology Service (Australia)
T.J. Samson Community Hospital (KY)
Taipei Veterans General Hospital (Taiwan)
Taiwan Society of Laboratory Medicine
Tallaght Hospital
Tartu University Clinics (Tartu)
Temple Univ. Hospital - Parkinson Pav. (PA)
Texas Children's Hospital (TX)
Texas Department of State Health Services
Thomason Hospital (TX)
Timmins and District Hospital (Canada)
The Toledo Hospital (OH)
Touro Infirmary (LA)
Tri-Cities Laboratory (WA)
Trident Medical Center (SC)
Trinity Medical Center (AL)
Tripler Army Medical Center (HI)
Tufts New England Medical Center Hospital (MA)
Tulane Medical Center Hospital & Clinic (LA)
Turku University Central Hospital
UCI Medical Center (CA)
UCLA Medical Center Clinical Laboratories (CA)
UCSD Medical Center (CA)
UCSF Medical Center China Basin (CA)
UMass Memorial Medical Center (MA)
UMC of Southern Nevada (NV)
UNC Hospitals (NC)
Union Clinical Laboratory (Taiwan)
United Christian Hospital (Hong Kong)
United Clinical Laboratories (IA)
Unity HealthCare (IA)
Universita Campus Bio-Medico (Italy)
Universitair Ziekenhuis Antwerpen (Belgium)
University College Hospital (Ireland)
University Medical Center at Princeton (NJ)
University of Alabama-Birmingham Hospital (AL)
University of Arkansas for Medical Sci. (AR)
University of Chicago Hospitals (IL)
University of Colorado Health Sciences Center (CO)
University of Colorado Hospital
University of Iowa Hospitals and Clinics (IA)
University of Kentucky Med. Ctr. (KY)
University of Maryland Medical System (MD)
University of Medicine & Dentistry, NJ University Hosp. (NJ)
University of Miami (FL)
University of Missouri Hospital (MO)
University of MN Medical Center - Fairview
University of MS Medical Center (MS)
University of So. Alabama Children's and Women's Hospital (AL)
University of Texas Health Center (TX)
The University of Texas Medical Branch (TX)
University of the Ryukyus (Japan)
University of Virginia Medical Center
University of Washington
UPMC Bedford Memorial (PA)
U.S.A. Meddac (Pathology Division) (MO)
UW Hospital (WI)
UZ-KUL Medical Center (Belgium)
VA (Asheville) Medical Center (NC)
VA (Bay Pines) Medical Center (FL)
VA (Chillicothe) Medical Center (OH)
VA (Cincinnati) Medical Center (OH)
VA (Dallas) Medical Center (TX)
VA (Dayton) Medical Center (OH)
VA (Decatur) Medical Center (GA)
VA (Hines) Medical Center (IL)
VA (Indianapolis) Medical Center (IN)
VA (Iowa City) Medical Center (IA)
VA (Long Beach) Medical Center (CA)
VA (Miami) Medical Center (FL)
VA New Jersey Health Care System (NJ)
VA Outpatient Clinic (OH)
VA (Phoenix) Medical Center (AZ)
VA (San Diego) Medical Center (CA)
VA (Seattle) Medical Center (WA)
VA (Sheridan) Medical Center (WY)
VA (Tucson) Medical Center (AZ)
Valley Health (VA)
Vancouver Hospital and Health Sciences Center (BC, Canada)
Vancouver Island Health Authority (Canada)
Vanderbilt University Medical Center (TN)
Via Christi Regional Medical Center (KS)
Virga Jessezieukenhuis (Belgium)
ViroMed Laboratories (LabCorp) (MN)
Virtua - West Jersey Hospital (NJ)
WakeMed (NC)
Walter Reed Army Medical Center (DC)
Warren Hospital (NJ)
Washington Hospital Center (DC)
Waterbury Hospital (CT)
Waterford Regional Hospital (Ireland)
Wayne Memorial Hospital (NC)
Weirton Medical Center (WV)
Wellstar Douglas Hospital Laboratory (GA)
Wellstar Paulding Hospital (GA)
Wellstar Windy Hill Hospital Laboratory (GA)
West China Second University Hospital, Sichuan University (P.R. China)
West Valley Medical Center Laboratory (ID)
Westchester Medical Center (NY)
Western Baptist Hospital (KY)
Western Healthcare Corporation (Canada)
Wheaton Franciscan & Midwest Clinical Laboratories (WI)
Wheeling Hospital (WV)
Whitehorse General Hospital (Canada)
William Beaumont Army Medical Center (TX)
William Beaumont Hospital (MI)
William Osler Health Centre (Canada)
Winchester Hospital (MA)
Winn Army Community Hospital (GA)
Wisconsin State Laboratory of Hygiene (WI)
Wishard Health Sciences (IN)
Womack Army Medical Center (NC)
Woodlawn Hospital (IN)
York Hospital (PA)

OFFICERS

Robert L. Habig, PhD,
President
Habig Regulatory Consulting

Gerald A. Hoeltge, MD,
President-Elect
Cleveland Clinic

Mary Lou Gantzer, PhD,
Secretary
Dade Behring Inc.

W. Gregory Miller, PhD,
Treasurer
Virginia Commonwealth University

Thomas L. Hearn, PhD,
Immediate Past President
Centers for Disease Control and Prevention

Glen Fine, MS, MBA,
Executive Vice President

BOARD OF DIRECTORS

Susan Blonshine, RRT, RPFT, FAARC
TechEd

Maria Carballo
Health Canada

Russel K. Enns, PhD
Cepheid

Lillian J. Gill, DPA
FDA Center for Devices and Radiological Health

Prof. Naotaka Hamasaki, MD, PhD
Nagasaki International University

Valerie Ng, PhD, MD
Alameda County Medical Center/
Highland General Hospital

Janet K.A. Nicholson, PhD
Centers for Disease Control and Prevention

Luann Ochs, MS
BD Diagnostics – TriPath

Timothy J. O'Leary, MD, PhD
Department of Veterans Affairs

Klaus E. Stinshoff, Dr.rer.nat.
Digene (Switzerland) Sàrl (Retired)

Michael Thein, PhD
Roche Diagnostics GmbH

James A. Thomas
ASTM International

940 West Valley Road ▾ Suite 1400 ▾ Wayne, PA 19087 ▾ USA ▾ PHONE 610.688.0100
FAX 610.688.0700 ▾ E-MAIL: customerservice@clsi.org ▾ WEBSITE: www.clsi.org ▾ ISBN 1-56238-665-4



CLINICAL AND LABORATORY STANDARDS INSTITUTE®
(Formerly NCCLS)